

MEDICAL ROBOTS

Telerobotic neurovascular interventions with magnetic manipulation

Yoonho Kim¹, Emily Genevriere¹, Pablo Harker^{2,3}, Jaehun Choe¹, Marcin Balicki⁴, Robert W. Regenhardt², Justin E. Vranic², Adam A. Dmytriw², Aman B. Patel², Xuanhe Zhao^{1,5*}

Copyright © 2022
The Authors, some
rights reserved;
exclusive licensee
American Association
for the Advancement
of Science. No claim
to original U.S.
Government Works

Advances in robotic technology have been adopted in various subspecialties of both open and minimally invasive surgery, offering benefits such as enhanced surgical precision and accuracy with reduced fatigue of the surgeon. Despite the advantages, robotic applications to endovascular neurosurgery have remained largely unexplored because of technical challenges such as the miniaturization of robotic devices that can reach the complex and tortuous vasculature of the brain. Although some commercial systems enable robotic manipulation of conventional guidewires for coronary and peripheral vascular interventions, they remain unsuited for neurovascular applications because of the considerably smaller and more tortuous anatomy of cerebral arteries. Here, we present a teleoperated robotic neurointerventional platform based on magnetic manipulation. Our system consists of a magnetically controlled guidewire, a robot arm with an actuating magnet to steer the guidewire, a set of motorized linear drives to advance or retract the guidewire and a microcatheter, and a remote-control console to operate the system under real-time fluoroscopy. We demonstrate our system's capability to navigate narrow and winding pathways both *in vitro* with realistic neurovascular phantoms representing the human anatomy and *in vivo* in the porcine brachial artery with accentuated tortuosity for preclinical evaluation. We further demonstrate telerobotically assisted therapeutic procedures including coil embolization and clot retrieval thrombectomy for treating cerebral aneurysms and ischemic stroke, respectively. Our system could enable safer and quicker access to hard-to-reach lesions while minimizing the radiation exposure to physicians and open the possibility of remote procedural services to address challenges in current stroke systems of care.

INTRODUCTION

Stroke remains one of the leading causes of death and long-term disabilities in the United States, where it kills about 140,000 people and costs around \$46 billion each year (1). Stroke occurs when blood flow to the brain is blocked by blood clots or plaques (ischemic) or when a weakened blood vessel ruptures and causes bleeding in the brain (hemorrhagic). Both ischemic and hemorrhagic strokes can lead to permanent brain damage, and hence, early intervention is critical to better protect the brain. However, current stroke systems of care require physically transporting patients to tertiary hospitals for such interventions. For patients in rural areas, where acute-care services are often unavailable, stroke is challenging to treat in a timely fashion, and patients can become no longer eligible for therapies when their brains are irreparably damaged. One potential solution to this logistical challenge is to use teleoperated robotic systems for remote surgery (2). Such telerobotic platforms could enable skilled neurointerventionalists (physicians who are surgically trained for endovascular stroke intervention) at large institutions to perform surgical tasks remotely on patients at their local hospitals, obviating transport of patients at the expense of time (3).

In the broader context of endovascular neurosurgery, there are several challenges in the operating room as well. In neurovascular

interventions, microguidewires are primarily used for intravascular access to target lesions and to facilitate the placement of other interventional or therapeutic devices, such as microcatheters, coils, and stents. For steering purposes, typical guidewires have preshaped or shapeable distal tips that can be oriented toward a desired direction by manually twisting their proximal ends. However, this twisting maneuver for conventional passive guidewires often becomes ineffective and rather unpredictable because of the jerky motion of the prebent tip caused by friction, also known as “whipping” (4), particularly when navigating through narrow and winding pathways. This makes it difficult to reach distal branches of cerebral arteries and in some circumstances renders distal target access unfeasible. The predefined shape of the tip might also deform within the vessel, especially during complicated and lengthy guiding maneuvers (5). Moreover, interventionalists often need to continuously turn the guidewire while inserting it to prevent the prebent tip from latching onto any small ostium or opening along the path; the distal tip could otherwise become stuck and potentially cause vascular injury or perforation upon further pushing. To avoid such complications, physicians always need to verify the distal tip movement under fluoroscopy when manually manipulating guidewires, which exposes them to continuous x-rays during the interventional procedures. For interventionalists, this repetitive radiation exposure is being recognized as a greater risk than previously appreciated (6, 7). Telerobotic interventional systems, which allow for remote control of robotic guidewires with active steering and navigational capabilities, could potentially help to resolve these clinical and technical challenges as well.

However, robotic applications to endovascular neurosurgery have remained largely unexplored because of the lack of appropriate

¹Department of Mechanical Engineering, Massachusetts Institute of Technology, Cambridge, MA, USA. ²Department of Neurosurgery, Massachusetts General Hospital and Harvard Medical School, Boston, MA, USA. ³Department of Neurology and Rehabilitation Medicine, University of Cincinnati College of Medicine, Cincinnati, OH, USA. ⁴Philips Research North America, Cambridge, MA, USA. ⁵Department of Civil and Environmental Engineering, Massachusetts Institute of Technology, Cambridge, MA, USA.


*Corresponding author. Email: zhaox@mit.edu

technologies. The biggest hurdle thus far has been the miniaturization of robotic devices so that they are thin and flexible enough to navigate through narrow and complex neurovasculature. Existing robotic catheters or endoscopes with active steering and navigational capabilities are often limited to relatively large scales (a few millimeters in diameter), because of the miniaturization challenges inherent in their conventional actuation mechanisms (8), and are therefore unsuitable for endovascular interventions (9).

Instead of directly tackling the challenges of realizing robotic or steerable guidewires and catheters at submillimeter scale, the industry has developed vascular robotic platforms that can accommodate and manipulate conventional guidewires and catheters under remote control. For example, the Magellan Robotic System of Hansen Medical (acquired by Auris Health) features an articulating sheath with linear and rotary drives to enable insertion, rotation, and retraction of conventional guidewires (9, 10). Other examples include the CorPath GRX of Corindus Vascular Robotics (acquired by Siemens Healthineers) and R-One of Robocath, both of which can similarly advance or retract and rotate commercially available guidewires and catheters using linear and rotary drives under remote control (11). The R-One system has recently been approved for percutaneous coronary intervention only in the European Union (12), and the CorPath GRX is currently approved for peripheral vascular intervention as well as percutaneous coronary intervention in the United States, European Union, and other countries (13). Although the CorPath GRX was originally designed to manipulate the larger-gauge devices used for percutaneous coronary and peripheral vascular interventions, the system is cleared for neurovascular intervention in the European Union, Australia, and New Zealand (13). However, it has not yet been approved for neurovascular intervention in other countries, including the United States (14), possibly because of its current technical limitations for intracranial applications as discussed in a recent report (15). After some modifications in the system to facilitate the use of smaller guidewires and microcatheters for intracranial access and intervention, recent publications reported its first-in-human, off-label use for endovascular coiling of aneurysms in relatively proximal areas of the intracranial artery (13, 16). However, to date, no robotic systems have been reported to accomplish robotically assisted endovascular treatment of cerebral aneurysms or infarctions that commonly occur in more distal and difficult-to-reach areas such as the middle cerebral artery (MCA) or anterior cerebral artery (ACA). The existing robotic systems designed to manipulate conventional guidewires would retain the functional limitations inherent in the twist-based steering of preshaped, passive guidewires discussed above.

The present work is aimed at tackling the aforementioned technical and clinical challenges in current endovascular neurosurgery and stroke systems of care, where the application of robotics can be the key to the solution. Here, we present a teleoperated magnetic manipulation platform to enable robotic

application in endovascular neurosurgery for treating stroke and aneurysms (Movie 1), which has remained largely unattainable with existing continuum or vascular robotic systems. Our telerobotic neurointerventional system allows for precise control of a magnetically steerable, soft continuum guidewire in the complex neurovasculature through a robot arm with an actuating magnet attached to its end effector that is remotely controlled by an operator to apply the magnetic fields required for actuation and steering of the magnetic guidewire. A pair of motorized linear drives can advance or retract the guidewire, and a microcatheter can travel over the guidewire along the navigated path. Through quantitative analysis and characterization of the magnetic guidewire's behavior under the action of the actuating magnet, we identified a set of fundamental and unique steering control principles for the magnetic soft continuum guidewire that can provide guidance on how to manipulate the single actuating magnet with minimal motion of the robot arm to achieve the desired configuration of the guidewire. Through real-time teleoperation of the system under feedback from x-ray fluoroscopy and virtual visualization of the robot arm, we demonstrate our system's steering and navigational capabilities to enable access to different branches of cerebral arteries using realistic anatomical models that include all relevant pathway attributes to represent the human neurovascular anatomy. We further demonstrate our system's capability to telerobotically assist therapeutic procedures that are commonly performed in endovascular neurosurgery, such as coil embolization for treating cerebral aneurysms and clot retrieval thrombectomy for treating ischemic stroke due to cerebral infarctions. Then, to validate the safety and effectiveness of our system in physiologically relevant conditions, we demonstrate the system's steering and navigational capabilities in vivo using a porcine brachial artery tortuosity model (17) that simulates the tortuosity of the human intracranial arteries. Last, to evaluate the user experience with our developed system, we assess the learning curve for neurointerventionalists associated with real-time teleoperation of the system for magnetic steering and navigation in vitro with clinically challenging anatomy.

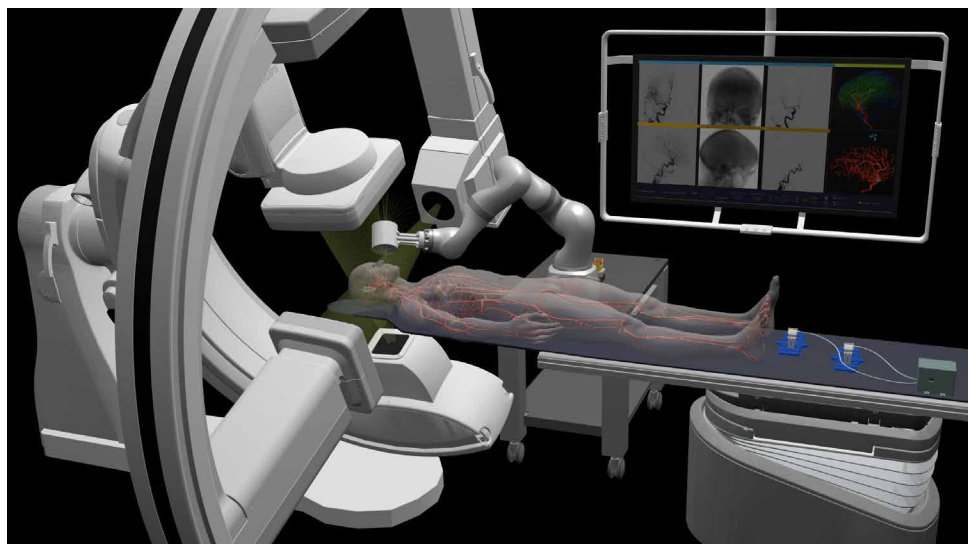

Movie 1. Overview of telerobotic stroke intervention based on magnetic manipulation.

RESULTS

Telerobotic system design overview

Figure 1 provides an overview of our telerobotic neurointerventional system deployed in clinical settings for image-guided endovascular procedures, with a C-arm fluoroscope providing real-time imaging of the guidewire navigating in the patient's blood vessels under magnetic manipulation. Mounted on a mobile platform beside the operating table, the robot arm is teleoperated by the interventionalist from a remote-control console to steer the magnetic guidewire by varying the position and orientation of the magnet at the robot arm's end effector around the patient's head. The guidewire/microcatheter advancing unit is placed near the patient to advance or retract the guidewire and the microcatheter from their proximal ends through the femoral or radial artery access point.

The magnetic guidewire has a steerable distal portion, which can be manipulated through spatial positioning of the actuating magnet at the robot arm's end effector relative to the steerable tip (Fig. 2A). Although spatial positioning of the magnet requires at most six degrees of freedom (DOFs), our system uses a 7-DOF serial robot arm manipulator with seven revolute joints (Fig. 2A) to take advantage of its kinematic redundancy for safer operation in cluttered environments with a confined workspace. The extra DOF provides an increased level of dexterity that helps the robot arm avoid singularities and joint limits (18) as well as workspace obstacles (the patient, C-arm, operating table, and radiation shields). The guidewire and the microcatheter can be advanced or retracted individually by a pair of advancing units, each of which uses a worm drive to convert the rotary motion transmitted from the DC motor at the base through a flexible shaft to a linear motion (Fig. 2A). The system is teleoperated from the remote-control console under visual feedback from

real-time fluoroscopic imaging of the guidewire/microcatheter in the blood vessels (Fig. 2B). The configuration of the robot arm is visualized in real time on the control workstation based on the joint position data (Fig. 2B). This real-time visualization helps the operator observe the current state of the robot arm while controlling it remotely. It can also be used for preprocedural planning and/or training of the robot manipulation in a virtual environment replicating the real world [three-dimensional (3D) computer-aided design models], including the surrounding objects that are known a priori, to help prevent collisions during operation while performing magnetic steering and navigation. Spatial positioning of the actuating magnet can be achieved via 6-DOF position control of the robot arm's end effector with a joystick controller, and advancement or retraction of the guidewire and the microcatheter can be controlled either independently or simultaneously with the joystick buttons (Fig. 2C). The operator could observe and confirm the current states of the guidewire and the microcatheter from the fluoroscopic images while operating the robot arm and the guidewire/catheter advancing units with the joystick controller from the remote-control console (Fig. 2B).

Design of the magnetic soft continuum guidewire

Leveraging our previous work on the design and fabrication of ferromagnetic soft continuum robots (8), we designed our magnetic guidewire to have a smaller outer diameter (400 μm) with greatly improved mechanical robustness in terms of both strength and toughness while maintaining good steerability. With these improvements, the newly designed magnetic guidewire is as thin and flexible as standard neurovascular guidewires and compatible with commercially available microcatheters for neurovascular interventions. The

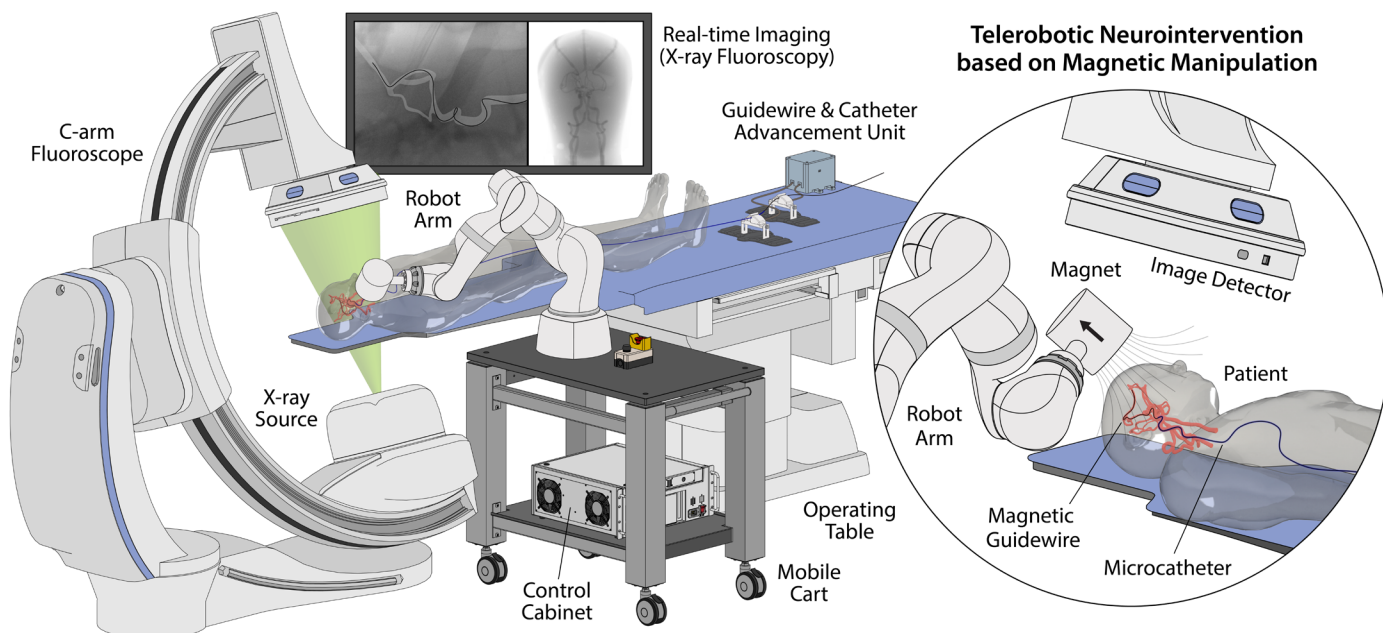


Fig. 1. Overview of the telerobotic neurointerventional platform based on magnetic manipulation. The system features a lightweight, compact robot arm with an actuating magnet attached to its end effector to remotely control a magnetically steerable guidewire through spatial positioning of the magnet around the patient's head. Mounted on a mobile platform beside the operating table, the robot arm is teleoperated from a remote-control console to steer the magnetic guidewire under real-time fluoroscopic imaging. The system further integrates a guidewire/microcatheter advancing unit based on a pair of motorized linear drives that can advance or retract the guidewire and a microcatheter upon remote control.

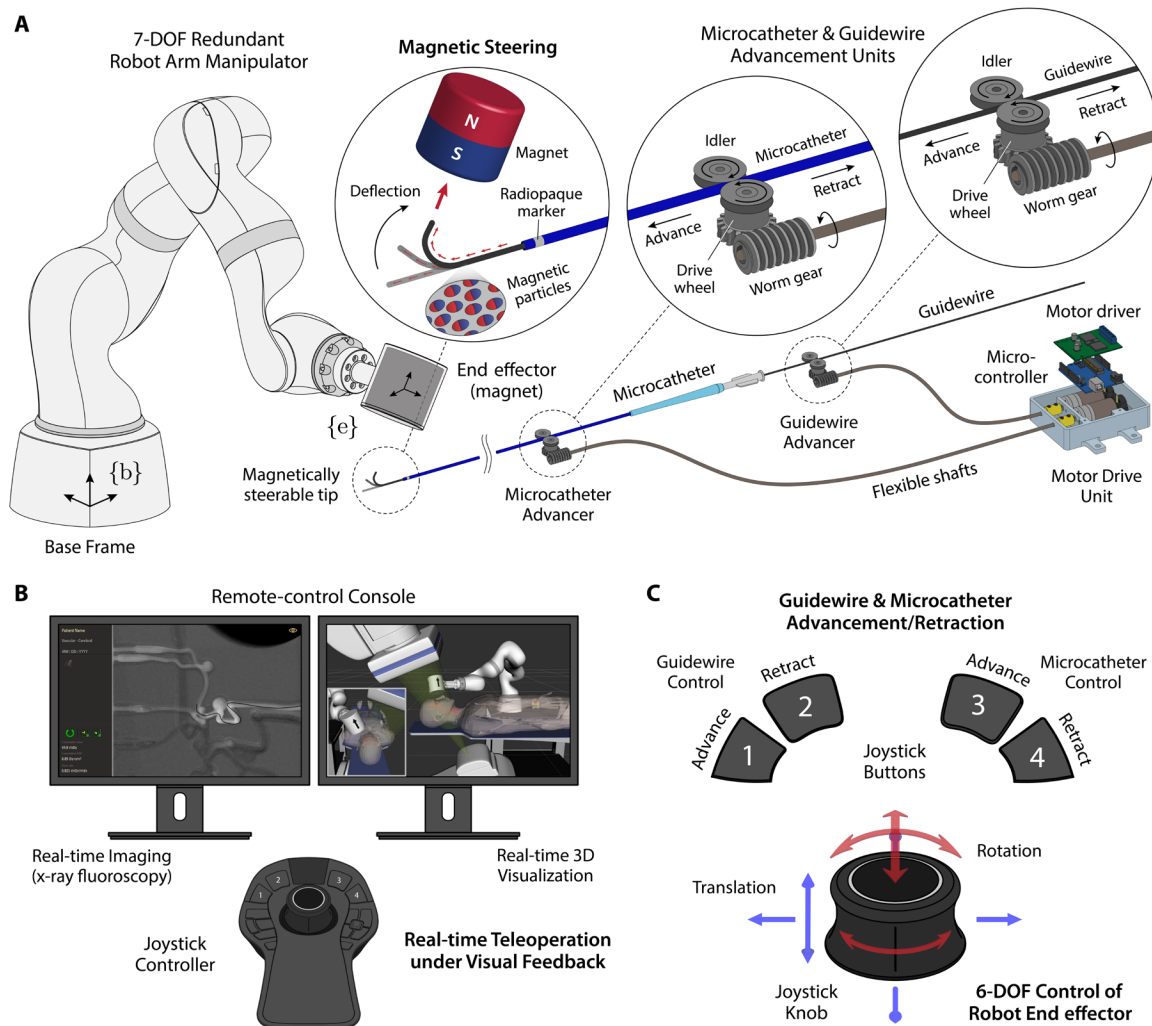


Fig. 2. Description of the telerobotic neurointerventional system. (A) The robot arm has 7 DOFs with kinematic redundancy for flexible manipulation and safer operation in cluttered environments. The guidewire has a magnetically responsive tip that contains magnetic particles and hence can be steered by the actuating magnet at the robot arm’s end effector. The guidewire is compatible with a standard microcatheter that travels over the guidewire along the navigated path. The guidewire and the microcatheter can be advanced/retracted by a pair of advancing units, each of which uses a worm drive to convert the rotary motion of the DC motor at the base to a linear motion. (B) The system is teleoperated from the remote-control console under feedback from real-time imaging of the guidewire/microcatheter in the blood vessels and virtual visualization of the robot arm. The magnetic guidewire is naturally visible under x-ray because of the embedded magnetic particles, and the position of the microcatheter can be identified by the radiopaque marker at the distal end. The robot arm is visualized in a virtual environment that replicates the real world on the control workstation to allow the operator to avoid collisions with surrounding objects while teleoperating the robot arm. (C) Spatial positioning of the magnet is achieved via 6-DOF position control of the robot arm’s end effector with a joystick controller, and advancement/retraction of the guidewire and the microcatheter can be controlled either independently or simultaneously with the joystick buttons.

magnetic guidewire consists of a tapered core of nickel-titanium alloy (nitinol), which is coated with a soft, yet durable polymer jacket composed of thermoplastic polyurethane (TPU) with embedded neodymium-iron-boron (NdFeB) particles. With the NdFeB particles in the polymer jacket magnetized along the guidewire’s axial direction, the distal portion (50 mm from the end) of the guidewire is magnetically responsive and can be steered with an actuating magnet (Fig. 2A), using the magnetic torques and forces generated from the embedded magnetic dipoles under the applied fields and field gradients (19–21). The NdFeB particle loading concentration was determined to be 20% by volume according to the optimal design strategy proposed in the previous study (8). The

resultant magnetic polymer jacket has a magnetization (M) of 128 kA/m and a shear modulus (G) of 1210 kPa (fig. S1A).

To enable sharp turns at acute-angled corners in blood vessels with clinically challenging tortuosity, a short segment (4 mm long; denoted L_2 in Fig. 3B) at the distal end of the guidewire’s magnetically responsive portion is composed of the TPU-NdFeB composite only, without the stiff nitinol core, and is therefore much softer and more responsive than the remainder that contains the nitinol core. When magnetic fields are applied by the actuating magnet, the unconstrained portion (free from contact with blood vessels) of the guidewire’s steerable tip of length L , which consists of a stiffer segment of length L_1 that contains the nitinol core and the softer segment of

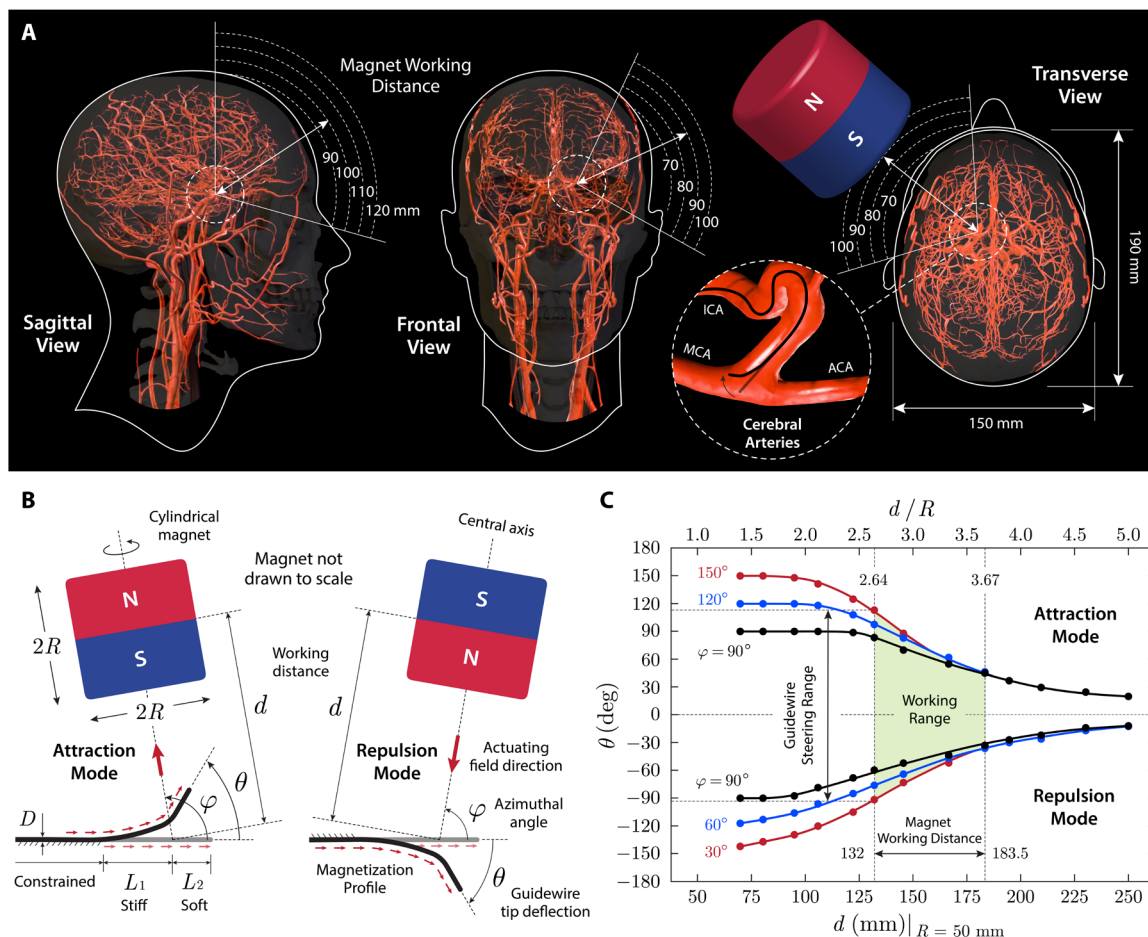


Fig. 3. Design considerations for magnetic steering with a single magnet. (A) Working distance and area for a cylindrical magnet (diameter and thickness of 100 mm) around the head considering the average head size (23) and anatomical location and orientation of intracranial arteries illustrated on the sagittal, frontal, and transverse planes. When viewed from the sagittal plane, the distance from the surface of the magnet to the circle of Willis in the middle of the head is estimated to be around 100 mm. When viewed from the frontal and transverse planes, the distance from the surface of the magnet to left ICA bifurcation is estimated to be 80 to 90 mm. (B) Attraction and repulsion modes for steering control of the magnetic guidewire with a single magnet of cylindrical shape (diameter and thickness of $2R$). The magnet working distance, denoted d , is defined as the distance from the center of the magnet to the base of the guidewire’s softer tip. The angular position of the magnet relative to the guidewire’s reference state is defined by the azimuthal angle φ , and the tip deflection angle is denoted θ . D indicates the outer diameter of the guidewire, and L_1 and L_2 denote the stiff and soft segments in the unconstrained (free to bend) portion of the guidewire’s steerable tip, respectively. (C) Characterization of the magnetic guidewire’s behavior under magnetic manipulation with a single magnet. The tip deflection angle θ was measured while varying the working distance and the angular position of the actuating magnet in the attraction and repulsion modes (guidewire dimension: $D=400\ \mu\text{m}$, $L_1=6\ \text{mm}$, $L_2=4\ \text{mm}$).

length L_2 that does not contain the stiff core, deflects either toward or away from the magnet depending on the magnetic polarity of the actuating magnet (Fig. 3B). Tensile strength testing demonstrated that the TPU-NdFeB composite can withstand tensile stresses up to 12 MPa, which translates into 1.5 N of tensile forces on the distal tip of the guidewire, while being stretched beyond 14 times its original length (fig. S1B). The measured tensile strength of the distal tip is comparable to that of commercially available neurovascular guidewires of similar dimension such as ASAHI CHIKAI 0.014-inch (360- μm) guidewires with a tensile strength of 2.45 N (22). However, the high stretchability of the TPU-NdFeB composite could provide greater resistance in terms of the energy required to cause fracture or joint failure at the distal tip when compared with conventional guidewires that typically have flexible spring or coil tips that are subject to brittle fracture.

Working distance for the actuating magnet

The use of a single actuating magnet for steering control of the magnetic guidewire requires some practical considerations when determining the shape, size, and working distance of the magnet, given the workspace constraints due to the patient geometry and surrounding objects as well as the spatial distribution of magnetic fields around the magnet. We first estimated a possible working range for the actuating magnet to steer the guidewire while it is spatially positioned near the patient’s head, with considerations of the average head size (23) and the anatomical location and orientation of intracranial arteries (Fig. 3A). For guidewire navigation in cerebral arteries, it is reasonable to consider the distance from the surface of the magnet to the circle of Willis—an arterial network in the middle of the head (between the right and left hemispheres; fig. S2A for vascular anatomy and nomenclature)—which can be regarded

as the farthest area within the cranium from the actuating magnet. Assuming that the magnet is positioned in one of the nearest possible locations around the head with some safety margins considered, the estimated distance from the magnet surface to the circle of Willis is around 100 mm, as illustrated on the sagittal plane in Fig. 3A. Then, for navigation from the proximal to the distal areas of cerebral arteries, the effective working distance between the magnet surface and the guidewire’s steerable tip would be below 100 mm and further decrease as the guidewire is advanced to the periphery. For example, if the guidewire is currently in the distal end (C4 in fig. S2B) of the left internal carotid artery (ICA; fig. S2B) and about to navigate through the left MCA (see fig. S2B), the estimated working distance from the magnet surface to the guidewire at the ICA bifurcation is around 80 to 90 mm, as illustrated on the frontal and transverse planes in Fig. 3A. Then, the magnetic field applied from this distance by the magnet should be strong enough to induce the deflection of the guidewire tip along the desired direction toward the left M1 segment (fig. S2B for vascular anatomy and nomenclature). To ensure this, we characterized the behavior of the steerable tip under the influence of applied magnetic fields and field gradients from a single actuating magnet in the following section.

Steering principles for the magnetic guidewire

Under spatially uniform magnetic fields (between a pair of magnets), magnetic steering of the guidewire is driven solely by magnetic torques, which cause the guidewire’s distal tip to bend toward the applied field direction (8, 20, 21). Magnetic actuation under spatially nonuniform fields (e.g., with a single magnet), however, involves magnetic forces as well as magnetic torques because of the presence of field gradients (8, 21). Therefore, the effects of magnetic forces on the guidewire’s behavior should also be characterized when designing the steering control interface based on magnetic manipulation with a single magnet. Under the actuating magnetic field denoted by a vector \mathbf{B} , with the magnetization of the guidewire tip along its axial direction denoted by a vector \mathbf{M} , the magnetic body torque density (per unit volume of the magnetic composite material) can be expressed as

$$\boldsymbol{\tau} = \mathbf{M} \times \mathbf{B} \quad (1)$$

and the magnetic body force density (per unit volume of the magnetic composite material) as

$$\mathbf{b} = (\text{grad}\mathbf{B})\mathbf{M} \quad (2)$$

where $\text{grad}\mathbf{B}$ denotes the spatial gradient of the applied magnetic field.

For the actuating magnet, we consider an axially magnetized, NdFeB (N52-grade) magnet of cylindrical shape (diameter and thickness of $2R$; Fig. 3B) with an axisymmetric field distribution (fig. S3A). For cylindrical magnets with the same diameter-to-thickness ratio, the shape of the magnetic field remains the same when normalized by the magnet’s characteristic dimension (e.g., radius R). Therefore, the magnetic field at a certain point around the magnet can be expressed as a vector function of the spatial location of the point (denoted by a position vector \mathbf{p} with respect to the center of the magnet in cylindrical coordinates) in a normalized form (by the magnet radius R) as

$$\mathbf{B}(\mathbf{p}) = B_{re} \mathcal{F}(\mathbf{p}/R) \quad (3)$$

where B_{re} is the remanence of the magnet and \mathcal{F} denotes the vector function whose implicit form can be found in (24–26). Along the central axis of the magnet, the magnitude of the magnetic field can be expressed explicitly in a normalized form as

$$B = \frac{B_{re}}{2} \left(\frac{d/R + 1}{\sqrt{(d/R + 1)^2 + 1}} - \frac{d/R - 1}{\sqrt{(d/R - 1)^2 + 1}} \right) \quad (4)$$

where d is the distance from the center of the magnet to the point of interest/measurement along the centerline (i.e., $\pm z$ direction in fig. S3A). Because the magnetic field strength decreases with the normalized distance d/R , as shown in fig. S3B, the actuating magnet should be large enough to steer the guidewire at a reasonable working distance discussed above. Typical steering and navigational tasks require the actuating field strength of at most 80 mT (8), which corresponds to the flux density at $d/R = 2.64$ from the center of the magnet as predicted from Eq. 4 and shown in fig. S3B. For a cylindrical magnet with diameter and thickness of 100 mm (i.e., $R = 50$ mm) and $B_{re} = 1.45$ T, for example, this normalized distance translates into 132 mm from the magnet’s center (or 82 mm from the magnet’s surface). At this point, the field gradient along the centerline is calculated to be 1.75 mT/mm from the derivative of Eq. 4 as shown in figs. S3C and S4. Then, the magnetic torque density is evaluated to be 10.24 kN/m² from Eq. 1, and the moment acting on the guidewire’s steerable tip of length L ($4 \leq L \leq 10$ mm) by the magnetic body force (per unit volume) is estimated from Eq. 2 to be 0.90 to 2.24 kN/m², which is around 10 to 20% of the magnetic torque density. The contribution of the magnetic body force to the steering of the distal tip further diminishes as the magnet size increases (i.e., inversely proportional to R ; see fig. S3C), when compared with that of the magnetic torque. This implies that, for the magnetic guidewire, the magnetic torques are still the primary source of actuation even when it is steered by a single permanent magnet, provided that the actuating magnet is much larger than the steerable tip of the guidewire (i.e., $R \gg L$) and sufficiently far from the guidewire tip ($d > 2R$). Under these conditions, the tip deflection behavior of the guidewire can be characterized as a function of the normalized working distance from the magnet.

Principal modes of steering control

The most straightforward way to steer the magnetic guidewire with a single magnet is to position the magnet in such a way that the guidewire’s distal tip bends toward the magnet. Such wire tip motion can be achieved by aligning the magnet’s magnetic moment, which points from the south to the north pole of the magnet along its central axis, with the desired steering direction to which the tip deflection is to occur. We define this mode of steering control, which seemingly attracts the distal end of the guidewire, as the attraction mode (Fig. 3B). If the magnet is flipped, with its magnetic moment reversed, the guidewire tip would be repelled away from the magnet surface. By the same token, we define this mode of steering control as the repulsion mode (Fig. 3B). We define the angular position of the magnet relative to the guidewire by the azimuthal angle (denoted φ in Fig. 3B), which is the angle formed by the line connecting the base of the guidewire’s softer tip in the undeformed reference state and the center of the magnet with respect to the straight tip of the guidewire. The working distance of the magnet is defined as the distance from the base of the guidewire’s softer tip in the reference state to the center of the magnet (denoted d in Fig. 3B).

The tip deflection angle (denoted θ in Fig. 3B) varies with the working distance (Fig. 3C), which is normalized by the magnet's radius R for nondimensional representation as discussed above. The deflection angle also varies with the magnet's angular position φ , helping to achieve larger deflection when φ is greater than 90° in the attraction mode or smaller than 90° in the repulsion mode, respectively (Fig. 3C). Note that the asymmetry between the attraction and repulsion modes is attributed to the influence of magnetic forces resulting from the spatial gradients of the actuating fields discussed above. In both the attraction and repulsion modes, the bending actuation is initiated and driven by the magnetic body torques because the magnetic body forces are almost negligible in the initial undeformed configuration (8). As the guidewire tip deforms and becomes more aligned with the applied fields, the magnetic body forces increase and attract the guidewire tip toward the magnet in both steering modes, as can be anticipated from Eq. 2. Consequently, the magnetic body forces help to increase the tip deflection angle in the attraction mode while decreasing the deflection angle in the repulsion mode, which leads to the slightly asymmetric profiles of the tip deflection angle as presented in Fig. 3C. Transition between the attraction and repulsion modes can be achieved through flipping the magnet by rotating the axis 7 of the robot arm by 180° (fig. S5A). Characterization of the guidewire's behavior during the transition (fig. S5B) is discussed in the Supplementary Materials.

Additional mode of steering control

Although the attraction and repulsion modes serve as the primary steering modes because of the intuitive control principles, they may not suffice for every possible case, especially when navigating in areas with unfavorable vascular anatomy for spatial positioning of the magnet due to workspace constraints. For such occasions, in which minimal motion of the robot arm is desirable, steering control of the magnetic guidewire can also be achieved through rotation of the magnet around its center, which corresponds to rotation of the end effector around the axis 7 of the robot arm. We define the rotation angle (denoted α in fig. S6A) as the deviation of the central axis of the magnet from its unrotated state, in which the magnet is positioned at the zero angular position ($\varphi = 0$) with its axis aligned with the undeformed (straight) tip of the guidewire from some working distance d (fig. S6A). The tip deflection angle θ varies with the magnet's rotation angle α ranging from -180° to 180° , as well as the normalized working distance d/R , as characterized in fig. S6B. When the magnet rotates clockwise ($\alpha < 0$) from the unrotated state, the guidewire tip bends counterclockwise ($\theta > 0$); when the magnet rotates counterclockwise ($\alpha > 0$), the guidewire tip bends clockwise ($\theta < 0$), just as two meshed gears turn in opposite directions. For the magnet positioned at either $-135^\circ < \alpha < -90^\circ$ or $90^\circ < \alpha < 135^\circ$, we define another useful steering mode, so-called the oblique repulsion mode (fig. S6A), which helps to deflect the guidewire tip up to around 90° at the normalized working distance of 2.64 (fig. S6B).

Size of the actuating magnet

The mappings between the position and orientation of the magnet and the behavior of the guidewire's distal tip presented in Fig. 3C and fig. S6B provide guidance on how to manipulate the magnet to achieve desired states of the guidewire. We define the range of working distances for the magnet in the attraction/repulsion mode as $2.64 \leq d/R \leq 3.67$ in terms of the normalized distance (Fig. 3C). The lower and upper boundaries correspond to the points along the

central axis of the magnet at which the magnetic flux density is 80 and 30 mT, respectively, according to Eq. 4 (fig. S3B). Within this range, the tip deflection angle can reach up to around 120° in the attraction mode and around 90° in the repulsion mode as shown in Fig. 3C. If we allow the magnet to approach the patient's head as close as 70 mm (in terms of the distance from the magnet surface to the target vasculature) in the scenario discussed above (Fig. 3A), the size of the smallest possible magnet is calculated to be around 85 mm in terms of both diameter and thickness ($R = 42.5$ mm). If we increase the minimum allowable distance (between the magnet surface and the target vasculature) to 85 mm, including some safety margins (around 20 mm from the head surface), the required diameter/thickness of the magnet becomes around 100 mm ($R = 50$ mm), which is considered the ideal size of the magnet to be used in realistic clinical settings. Hence, a cylindrical magnet with a size of 100 mm was used and mounted on the most distal joint/link of the robot arm with its magnetic moment aligned perpendicularly to the joint axis.

Teleoperation interface for the robot arm

Our teleoperation interface enables spatial positioning of the magnet through real-time position control of the robot arm's end effector using a joystick controller with a 6-DOF knob with which the operator can intuitively manipulate the actuating magnet as illustrated in fig. S7A. We describe the configuration of the robot arm using a joint-space vector $\mathbf{q} \in \mathbb{R}^7$ that represents the joint angles of the seven revolute axes. The position and orientation of the end-effector frame ($\{e\}$ in Fig. 2A) relative to the robot arm's base frame ($\{b\}$ in Fig. 2A) are defined by a task-space vector $\mathbf{x} \in \mathbb{R}^6$ with its first three components representing the position and the last three components representing the orientation. The differential kinematics, or the relation between the small change in the joint positions $\delta\mathbf{q}$ and the corresponding change in the end-effector pose $\delta\mathbf{x}$, can then be written as

$$\delta\mathbf{x} = \frac{\partial \mathbf{f}(\mathbf{q})}{\partial \mathbf{q}} \delta\mathbf{q} = \mathbf{J}(\mathbf{q}) \delta\mathbf{q} \quad (5)$$

where $\mathbf{J}(\mathbf{q}) \in \mathbb{R}^{6 \times 7}$ is the Jacobian or the partial derivatives of the forward kinematics defined by a mapping $\mathbf{x} = \mathbf{f}(\mathbf{q})$ with \mathbf{f} denoting a nonlinear vector function. Upon the operator's joystick manipulation, 6-DOF motion commands are produced as a combined set of incremental motions (translations and rotations) in each DOF, which are scaled and converted into the end effector's linear and angular motions in the task-space coordinates. The motion commands for the end effector $\delta\mathbf{x}$ are then transformed into the joint commands $\delta\mathbf{q}$ by multiplying the pseudo-inverse of the Jacobian $\mathbf{J}^\dagger(\mathbf{q})$

$$\delta\mathbf{q} = \mathbf{J}^\dagger(\mathbf{q}) \delta\mathbf{x} = \mathbf{J}^\top(\mathbf{q}) (\mathbf{J}(\mathbf{q}) \mathbf{J}^\top(\mathbf{q}))^{-1} \delta\mathbf{x} \quad (6)$$

which returns the minimum-norm solution for redundant manipulators like the one used in the present work by minimizing the two-norm $\|\delta\mathbf{q}\| = \sqrt{\delta\mathbf{q}^\top \delta\mathbf{q}}$ (27). The joint commands are added to the current joint positions to get new joint position values, which are sent to the robot arm controller (i.e., control cabinet in Fig. 1) to execute the motion that achieves the desired configuration of the robot arm.

In vitro verification with anatomical models

For validation of the developed telerobotic neurointerventional platform, we evaluated its steering and navigational performance in vitro

with anatomical models that replicate the human intracranial arteries. As part of benchtop verification, we first demonstrated our system's capability to guide selective navigation in different branches of cerebral arteries in a 3D neurovascular phantom under real-time optical imaging (fig. S7B) through telerobotically controlled magnetic manipulation (fig. S7C), as presented in movie S1. The task was performed in the presence of virtual C-arm models implemented in the robot arm's task space to simulate the workspace constraints in clinical settings for complex neurovascular interventions under biplane fluoroscopy (fig. S7D). In addition to the C-arm models, a virtual human patient on the operating table was also modeled in the robot's task space to ensure that the robot arm manipulation could be performed without collisions. The 3D neurovascular phantom was accessed from the left ICA (fig. S8 for detailed vascular structure) with the magnetic guidewire and the microcatheter, which were advanced up to the left ICA bifurcation (A1-M1 junction) using the remotely

controlled advancing unit. After positioning the actuating magnet to direct the guidewire tip toward the A1 segment of the left ACA (fig. S8) through repulsive steering, as shown in fig. S7C (00:01), the guidewire was advanced up to the anterior communicating artery (ACoA; fig. S8) and then to the M1 segment of the right MCA, as shown in fig. S7B (00:03) and movie S1 (00:00 to 00:03). Then, the guidewire was magnetically steered and manipulated within the confined space of ACoA complex to selectively reach the right and left A2 segments, as shown in fig. S7B (00:14 to 00:39) and movie S1 (00:03 to 00:44), which demonstrates our system's capability to control the magnetic guidewire remotely and precisely to navigate distal branches in the complex cerebral vasculature.

Then, for testing in a more realistic setting, we used a human head phantom with cranial housing and intracranial arteries (Fig. 4, A and B) under real-time x-ray fluoroscopy. Given that the vasculature between the proximal intracranial ICA to the MCA bifurcation (fig. S2

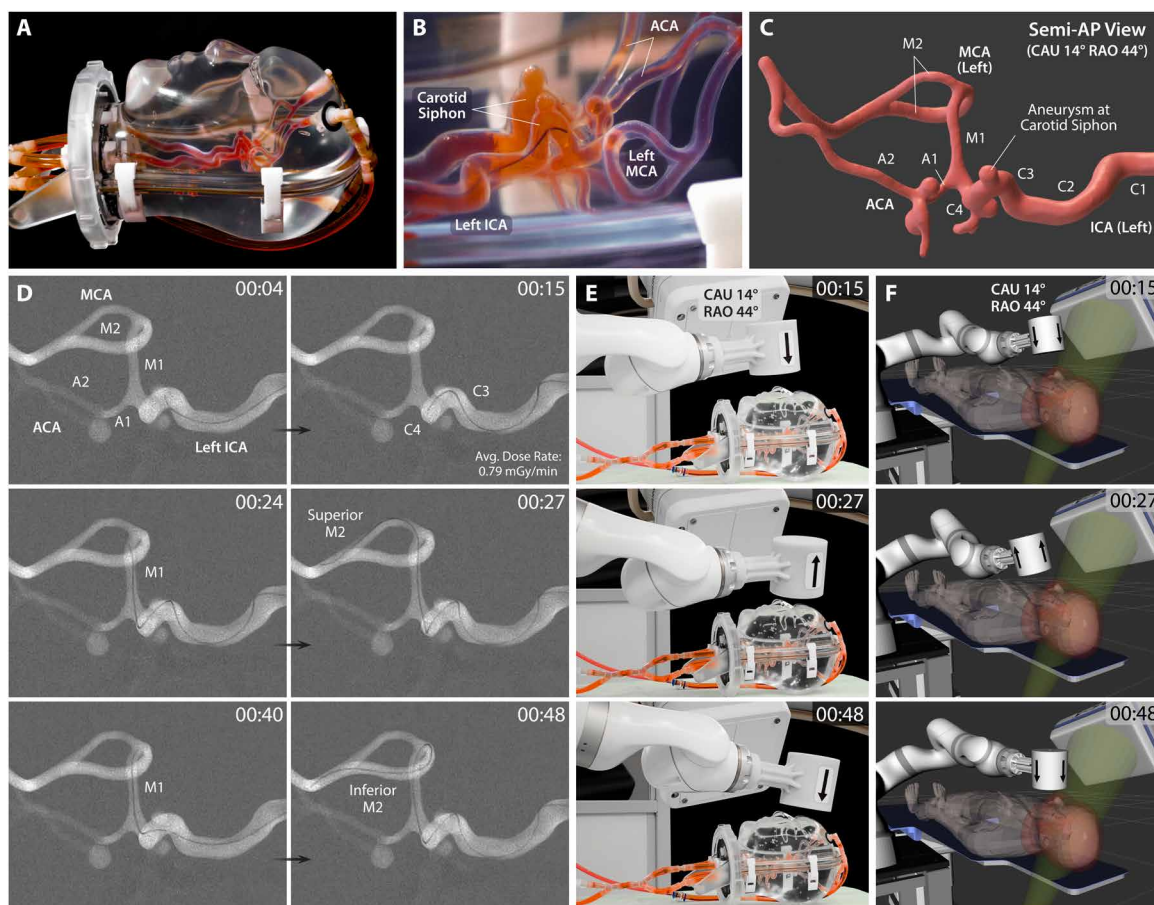


Fig. 4. In vitro demonstration of magnetic steering and navigation in intracranial arteries under real-time x-ray fluoroscopy. (A) Realistic human head phantom with replicated intracranial arteries based on silicone vessels. (B) Lateral view of the magnetic guidewire navigating in the left ICA with its distal tip being directed toward the descending portion of the carotid siphon under repulsive steering to avoid contact with the aneurysm at the apex of the carotid siphon. (C) Three-dimensional model of the target vasculature viewed from a semi-anteroposterior (AP) projection that shows all the important anatomical landmarks, including the carotid siphon with an aneurysm, the ICA bifurcation (A1-M1 junction), and the MCA bifurcation at the same time. (D) Fluoroscopic images of the magnetic guidewire navigating from the left ICA to MCA under telerobotically controlled magnetic steering to reach the superior and inferior M2 segments selectively in sequence. As part of the preprocedural step, digital subtraction angiography was performed to visualize the target vasculature as a roadmap for guidewire steering and navigation. (E) Actual view and (F) virtual visualization of the robot arm with an actuating magnet, the C-arm providing the semi-AP projection for the target vasculature in CAU 14° and RAO 44°, the human head phantom (or equivalently the virtual human patient) on the operating table. The arrow on the actuating magnet indicating the magnet's polarity identifies which steering mode is being used. A live fluoroscopy video is available in movie S2, which also shows the robot motion under real-time teleoperation in both the physical and virtual environments. The average time (\pm SD) it took for the demonstrated navigational task was 45.0 ± 4.0 s ($n = 5$).

for neurovascular anatomy) is the most common site for stroke or aneurysm intervention (6, 28), we chose to demonstrate magnetic steering and navigation in the left MCA of the phantom. First, to identify the 3D structure of the targeted vasculature, a series of images were obtained from 3D rotational angiography, and the data were reconstructed into a 3D vessel model (Fig. 4C) that allowed for a detailed view of the vascular structure from different perspectives. On the basis of the reconstructed 3D vascular model, a semi-anteroposterior projection was chosen to provide clear view of all the important anatomical landmarks along the path including the carotid siphon—the U-shaped part of the ICA between the cavernous (C3) and supraclinoid (C4) segments—with an aneurysm, the ICA bifurcation (A1-M1 junction), and the MCA bifurcation (M1-M2 junction), as annotated in Fig. 4C. The corresponding C-arm configuration, which is physically and virtually visualized in Fig. 4 (E and F, respectively), was with caudal angulation of 14° (CAU 14°) and right anterior oblique rotation of 44° (RAO 44°; fig. S9 for the C-arm nomenclature). The 3D vessel model was also used for preprocedural planning and simulation of the robot arm's motion, path, and configuration for spatial positioning of the actuating magnet to steer the magnetic guidewire at acute-angled corners or bifurcation points. The cranial housing of the head phantom (Fig. 4A) imposed realistic workspace constraints of the patient geometry (Fig. 3A). Again, the C-arm and the human patient models in the robot's virtual task space (Fig. 4F) helped to ensure that the robot manipulation could be performed without collisions.

As shown in Fig. 4D and movie S2, the magnetic guidewire was naturally visible under x-ray, as clearly as standard neurovascular guidewires, because of the embedded radiopaque magnetic particles. Starting from the left proximal ICA, the guidewire was first advanced to reach the carotid siphon, at which a saccular aneurysm (with an inner diameter of 4 mm) was present. As the guidewire entered the ascending part of the carotid siphon in the absence of magnetic steering, the straight tip of the guidewire was naturally directed toward the aneurysm (at the apex of the carotid siphon) as can be seen in Fig. 4D (00:04) and movie S2 (00:00 to 00:04). To prevent the guidewire tip from contacting the inner wall of the aneurysm upon further advancement, the actuating magnet was placed above the carotid siphon for repulsive steering (Fig. 4, E and F; 00:15), under which the guidewire tip was directed toward the descending segment of the carotid siphon so that it could pass the acute-angled corner without touching the aneurysm, as shown in Fig. 4D (00:15) and movie S2 (00:04 to 00:15). The guidewire was then further advanced up to the superior M2 segment under attractive steering at the ICA bifurcation (A1-M1 junction) to direct the distal tip toward the M1 branch, as shown in Fig. 4D (00:24 to 00:27) and movie S2 (00:15 to 00:27). The guidewire was then retracted back to the MCA bifurcation while flipping and repositioning the magnet for repulsive steering to reorient the guidewire tip toward the inferior M2 segment, after which the guidewire was advanced until it reached the end of the inferior M2 segment, as shown in Fig. 4D (00:40 to 00:48) and movie S2 (00:27 to 00:49).

This set of demonstrations with *in vitro* phantoms verifies that magnetic steering and navigation in intracranial arteries can be achieved with minimal motion of the actuating magnet through teleoperation of the system under visual feedback from real-time imaging and visualization in the presence of realistic workspace constraints. We also found that the magnetic guidewire could be steered effectively in the complex 3D vasculature without its view

for state observation being blocked or compromised by the actuating magnet. Given the steering principles based on a single magnet described in Fig. 3B and figs. S5A and S6A, it is unlikely that the view of the guidewire's steerable tip is blocked or interrupted by the actuating magnet during the steering task. This is because the plane of bending (on which the guidewire tip deflection is induced by the in-plane magnet motion) and the plane of view (on which the guidewire tip deflection is being observed) should be aligned with each other for optimal state observation. Hence, the argument that the magnet would not block the view of the guidewire tip during steering should generally hold for any vascular structure, provided that a suitable projection (the plane of view) was chosen for state observation of the guidewire in the target vasculature.

Telerobotically assisted aneurysm coil embolization

We further demonstrate our system's capability to telerobotically assist therapeutic procedures that are commonly performed in endovascular neurosurgery, such as coil embolization for treating intracranial aneurysms and clot retrieval thrombectomy for treating ischemic stroke. For endovascular treatments of aneurysms or stroke, therapeutic devices such as embolization coils or a stent retriever need to be delivered to the target lesion through a microcatheter. Aneurysms are localized points of vessel-wall weakening that create saccular or fusiform dilatations of the vessel wall, leading to risk of rupture (29). Intracranial aneurysms are typically treated endovascularly by deploying coils through a microcatheter to promote thrombosis within the aneurysm to eliminate blood flow into the dilated area, thereby reducing the risk of rupture (30). To demonstrate robotically assisted aneurysm coiling with our developed telerobotic neurointerventional platform, we used the same neurovascular phantom with multiple aneurysms (fig. S8) that was used for benchtop verification in fig. S7 and movie S1. The most distal (difficult-to-reach) aneurysms at the left and right MCA bifurcations (M1-M2 junctions) were chosen for demonstration.

To reach the target aneurysm at the left MCA bifurcation, the magnetic guidewire was first steered in the left ICA, where a large saccular aneurysm (with an inner diameter of 9 mm) was present in the carotid siphon (fig. S8). To cross the large gap within the aneurysm while avoiding contact with the inner wall of the aneurysm, the guidewire was manipulated under repulsive steering and advanced to the ICA bifurcation (A1-M1 junction) as shown in Fig. 5A (00:00 to 00:12) and movie S3 (00:00 to 00:15). Then, the guidewire was directed toward the left M1 segment to make a 90° turn under attractive steering, without touching the small aneurysm (with an inner diameter of 5 mm) located at the distal ICA (C4 in fig. S8A), and then advanced up to the target aneurysm (with an inner diameter of 7 mm) at the left MCA bifurcation (M1-M2 junction) as shown in Fig. 5A (00:24) and movie S3 (00:15 to 00:28). The guidewire was then directed toward the inferior M2 segment through repulsive steering to avoid touching the target aneurysm upon further advancement, as shown in Fig. 5A (00:34 to 00:38) and movie S3 (00:28 to 00:38). Then, the microcatheter was advanced up to the M1-M2 junction, after which the magnetic guidewire was retracted so that the microcatheter's distal tip could be placed inside the target aneurysm, as shown in Fig. 5A (00:46 to 00:55) and movie S3 (00:38 to 00:58). After full retraction and withdrawal from the microcatheter, the magnetic guidewire was replaced by an embolization coil device with its push wire engaged with the guidewire advancing unit. After the device exchange, the coil was advanced

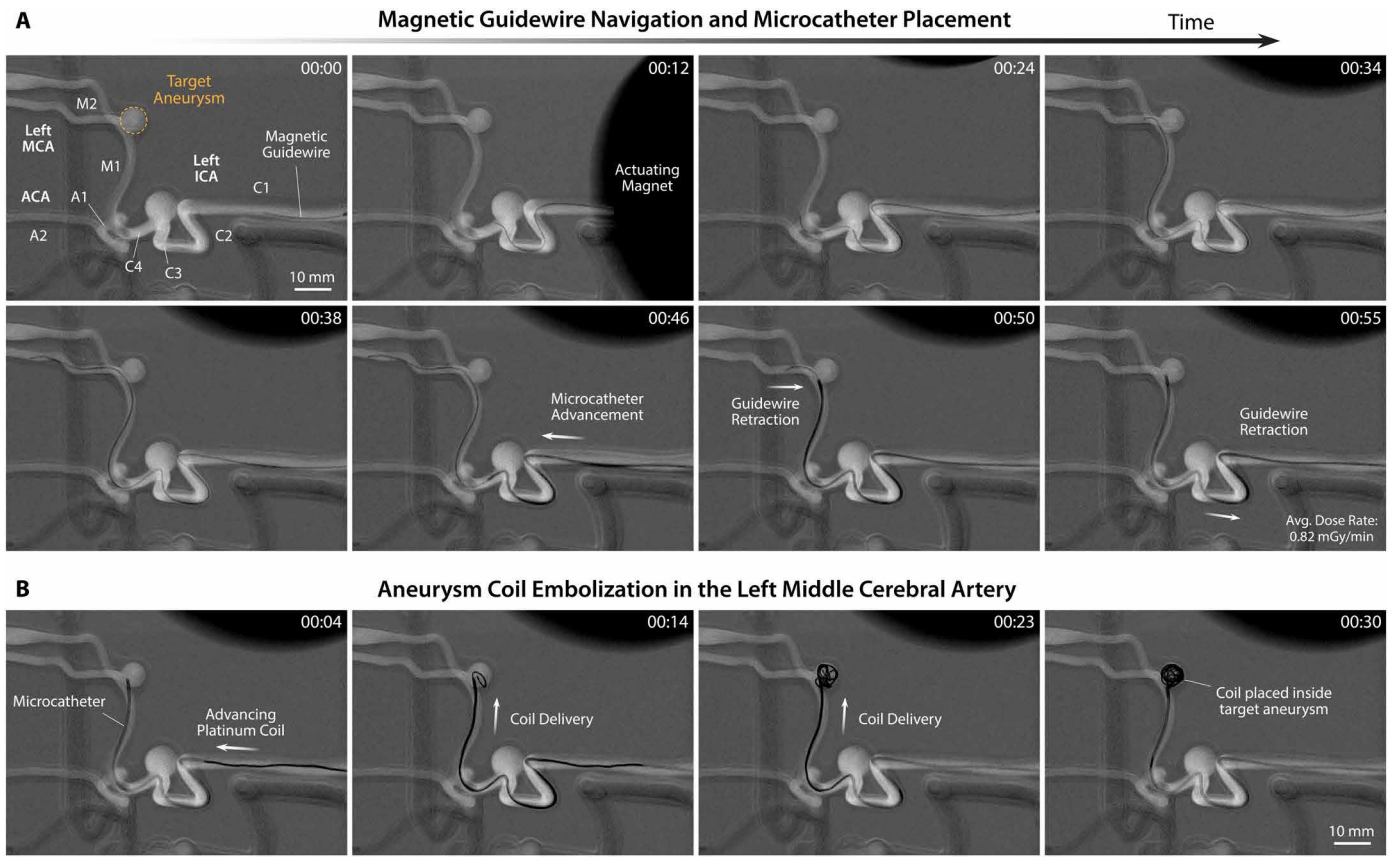


Fig. 5. Demonstration of telerobotically assisted aneurysm coil embolization in the MCA. (A) Magnetic steering and guidewire navigation up to the target aneurysm in the left MCA (00:00 to 00:38) and microcatheter placement in the target aneurysm sac while retracting the guidewire (00:46 to 00:55) through real-time teleoperation of the system under x-ray fluoroscopy. (B) Endovascular coiling of the targeted aneurysm by delivering embolization coils into the aneurysm sac through the placed microcatheter under joystick teleoperation of the advancing unit. Demonstration of the entire procedure from guidewire navigation and steering control to aneurysm coiling is presented in movie S3. The average time (\pm SD) it took for the demonstrated guidewire navigation and microcatheter placement in the targeted aneurysm in (A) was 51.7 ± 3.5 s ($n = 3$) and the coiling of the aneurysm in (B) was 32.3 ± 2.5 s ($n = 3$).

and delivered through the microcatheter into the target aneurysm under the joystick control of the advancing unit, as shown in Fig. 5B (00:04 to 00:30) and movie S3 (after 00:58). The real-time x-ray fluoroscopy confirmed successful coil placement in the target aneurysm.

We performed another aneurysm coiling with our telerobotic neurointerventional system in the most distal aneurysm at the right MCA bifurcation, as presented in fig. S10A and movie S4. Two large aneurysms were present in the neurovascular phantom (fig. S8), one with an inner diameter of 9 mm at the corner in the right ICA (C2) and the other with an inner diameter of 7.5 mm at the carotid siphon (C3-C4). Both of them imposed navigational challenges due to their presence at the acute-angled corners. The C-arm configuration was determined to provide a semilateral projection with CAU 18° and RAO 60° (fig. S9 for C-arm nomenclature). Starting from the proximal ICA, the guidewire was magnetically steered using the oblique repulsion mode to cross the first aneurysm without touching its inner wall and then advanced up to the second aneurysm as shown in fig. S10A (00:00 to 00:10) and movie S4 (00:00 to 00:15). Then, the guidewire tip was directed toward the distal ICA (C4) using repulsive steering to avoid contact with the second aneurysm, after which the guidewire was advanced until its distal tip reached

the right MCA bifurcation (M1-M2 junction), as shown in fig. S10A (00:30) and movie S4 (00:15 to 00:35). The guidewire was then further advanced to reach the inferior M2 segment under repulsive steering, as shown in fig. S10A (00:37 to 00:39) and movie S4 (00:35 to 00:39), which was to ensure that sufficient distance from the target aneurysm to the guidewire tip was reserved for smooth microcatheter advancement over the guidewire. The microcatheter was advanced up to the target aneurysm while retracting the guidewire so that the microcatheter tip could be placed in the aneurysm sac, after which the guidewire was completely withdrawn, as shown in fig. S10A (00:39 to 00:56) and movie S4 (00:39 to 00:58). An embolization coil was delivered through the microcatheter under the joystick control of the advancing unit until the aneurysm became densely packed with the coil, as shown in fig. S10B and movie S4 (after 00:58). These results presented in Fig. 5, fig. S10, and movies S3 and S4 demonstrate the potential of our developed platform for telerobotically assisted endovascular coiling of cerebral aneurysms to treat or prevent hemorrhagic stroke with potentially reduced operative time, perioperative risk, and radiation exposure. The results also illustrate the versatile applicability of our system to endovascular coiling procedures for treating intracranial aneurysms in hard-to-reach areas of the cerebral vasculature.

Telerobotically assisted clot retrieval thrombectomy

Next, we investigated the feasibility of our system for endovascular treatment of ischemic stroke due to cerebral infarction. For the feasibility test, we used a simulated, nonbiological blood clot to create occlusion in the M1 segment—one of the most common sites for a thrombus to lodge to cause cerebral ischemia (6)—in the right MCA of the same neurovascular phantom used for demonstrating the aneurysm coiling procedures. The artificial clot used in our experiment had similar mechanical and viscoelastic properties to a real blood clot (31). Given that the clot by itself was not visible under x-ray, the magnetic navigation and clot retrieval procedures were initially performed under real-time optical imaging to better visualize the whole process (x-ray results are also presented below), as shown in Fig. 6 and movie S5. Steering control and manipulation of the magnetic guidewire to the occluded site were similar to what was described for the previous demonstration of guidewire navigation in the same path presented in fig. S10A and movie S4, until the distal tip of the guidewire reached the clot, as shown in Fig. 6A (00:00 to 00:34) and movie S5 (00:00 to 00:34). The guidewire was further advanced so that the distal tip thrust itself into the tiny gap between

the clot and the vessel wall, under careful control of the guidewire advancing unit to avoid touching the inner wall of the first aneurysm at the corner, as shown in movie S5 (00:34 to 00:46). The guidewire tended to buckle inside the aneurysm upon further push, because of the high resistance from the clot, as can be seen in movie S5 (00:46 to 00:49). To avoid buckling by adding more mechanical support to the guidewire, the microcatheter was carefully advanced up to the clot while at the same time controlling the guidewire, after which the guidewire was advanced to pass through the artificial clot, as can be seen in Fig. 6A (01:35) and movie S5 (00:50 to 01:37). With the aid of magnetic steering of the guidewire at the MCA bifurcation, the microcatheter was placed across the occlusion such that its distal end was positioned distal to the thrombus, as shown in Fig. 6A (01:42) and movie S5 (01:38 to 01:49).

After withdrawing the guidewire, mechanical thrombectomy was performed to retrieve the clot using a commercially available revascularization device (i.e., a stent retriever; see Materials and Methods for details). Delivery of the stent retriever was performed manually following the standard procedure after inserting the stent introducer sheath into the hub of the microcatheter. The stent push

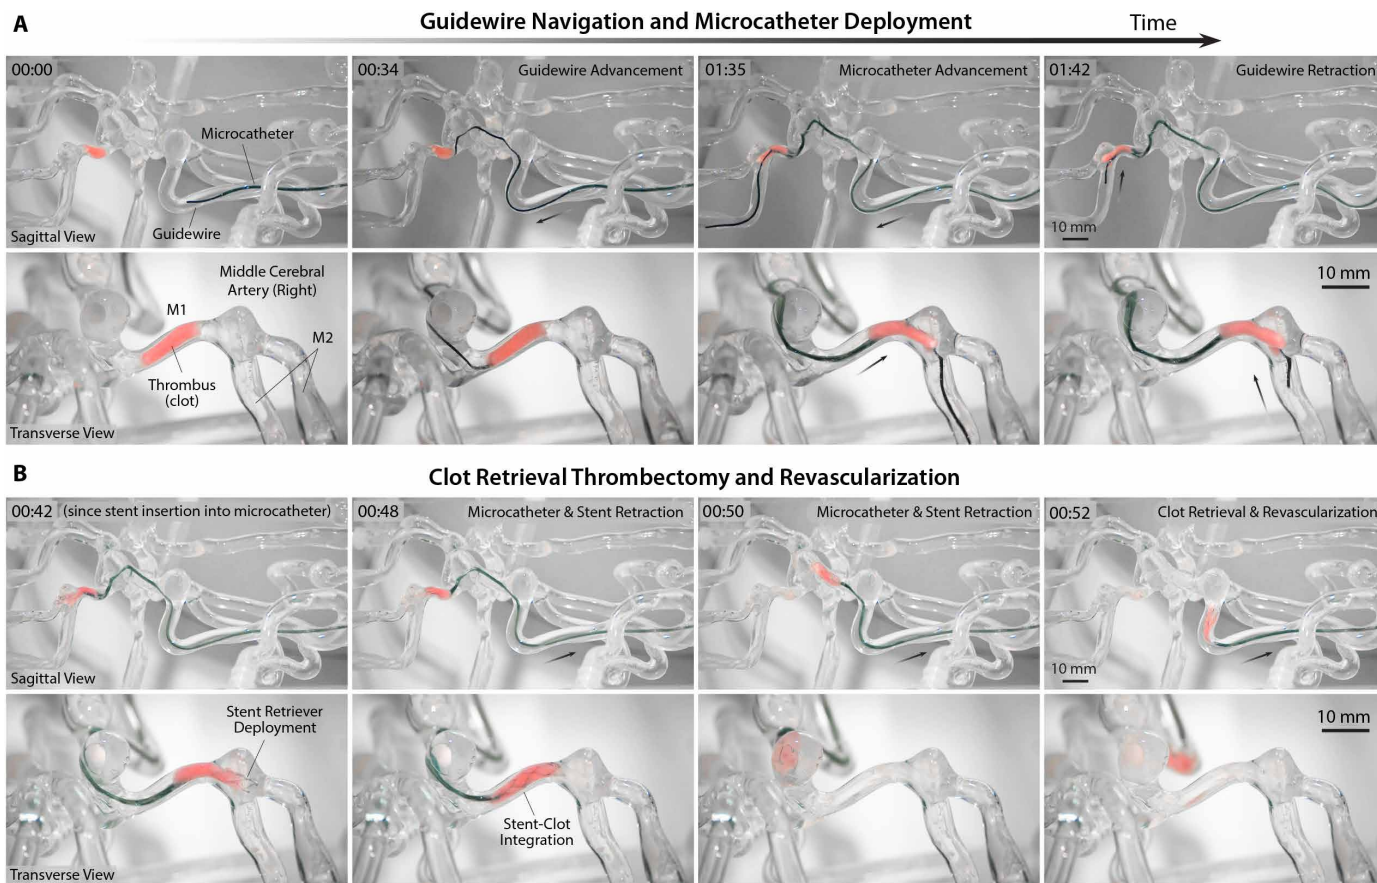


Fig. 6. Demonstration of telerobotically assisted clot retrieval thrombectomy and revascularization in the cerebral vasculature. (A) Navigation up to the simulated clot in the M1 segment of the right MCA with the telerobotically controlled magnetic guidewire (00:00 to 00:34) and microcatheter placement across the thrombus with the aid of magnetic steering at the MCA bifurcation (01:35 to 01:42) under real-time optical imaging to show the clot during the interventional process. (B) Deployment of a stent retriever across the thrombus (00:42 to 00:48) and retrieval of the clot upon withdrawal of the stent retriever and the microcatheter for revascularization of the occluded site (00:50 to 00:52). Demonstration of the entire navigation, steering control, and stent deploying procedures is available in movie S5. Telerobotically assisted clot retrieval procedure performed under real-time x-ray fluoroscopy is also presented in fig. S11. The average time (\pm SD) it took for the demonstrated guidewire navigation and microcatheter placement in the occluded site in (A) was 108.0 ± 14.0 s ($n = 3$) and the clot retrieval using the stent retriever in (B) was 46.7 ± 5.0 s ($n = 3$).

wire was advanced within the microcatheter until the distal markers of the stent retriever lined up with the distal end of the microcatheter, as shown in movie S5 (00:00 to 00:20 of the second part). Then, the microcatheter was carefully withdrawn under the joystick control of the catheter advancing unit while fixing the stent push wire to maintain the position of the stent until the distal end of the microcatheter was just proximal to the thrombus, thereby fully deploying the stent across the thrombus, as shown in Fig. 6B (00:42) and movie S5 (00:20 to 00:46). After confirming the stent deployment from the real-time imaging, the microcatheter and the stent as a unit were withdrawn to retrieve the clot and revascularize the occluded site (M1), as shown in Fig. 6B (00:48 to 00:52) and movie S5 (00:47 to 00:56).

We repeated the clot retrieval procedure under real-time x-ray fluoroscopy as shown in fig. S11 (A and B). Note that the infarcted right MCA was missing on the digital subtraction angiography (i.e., roadmap) images because of the occlusion in M1 blocking contrast flow (see corresponding optimal images in fig. S11, C and D), which is the same phenomenon observed in real stroke cases. The overall procedure and the workflow were similar to the previous demonstration in Fig. 6. However, greater distal migration of the clot was observed while advancing the guidewire and placing the microcatheter, as shown in fig. S11C (01:02 to 01:58), possibly because of the presence of pulsatile flow generated by the peristaltic pump. In contrast to the previous demonstration in which the stent retriever device was manually manipulated, this time we used the advancing unit and the joystick controller to manipulate both the stent retriever and the microcatheter when deploying the stent and retrieving the clot (fig. S11, B and D) to avoid radiation exposure during the procedures. Only the device exchange was done manually, after removing the guidewire from the microcatheter, by engaging the stent push with the guidewire advancing unit. The results presented in Fig. 6 and fig. S11 demonstrate the potential of our system for telerobotically assisted clot retrieval thrombectomy for treating ischemic stroke.

In vivo validation with porcine artery model

The series of in vitro verification results presented above have demonstrated our system's steering and navigational capabilities in clinically relevant settings for image-guided neurointervention using x-ray fluoroscopy, with realistic workspace constraints for the robot arm taken into account. The phantom studies allowed us to assess the physical and mechanical properties of the magnetic guidewire—such as radiopacity, stiffness, lubricity, and durability—in addition to the steering performance in the simulated human neurovascular anatomy with clinically challenging tortuosity and disease states. Although indispensable, performance evaluation in vitro based on anatomical models in general does not fully characterize all clinical experiences, outcomes, and risks (4). To verify our system's steering and navigational performance under realistic in vivo conditions while assessing the viscoelastic and physiological responses of blood vessels during the endovascular manipulation, we conducted animal testing using a porcine model.

Although pigs have been considered as excellent experimental animals for medical research because of the similarities between human and porcine biology (32), their head and neck geometry and intracranial arterial anatomy are quite different from those of humans. For example, in the pig exists a small and dense network (plexus) of interconnected vessels called rete mirabile, from which the ICA originates intracranially. Furthermore, the porcine intracranial arteries are much smaller in diameter (around 1 mm or less)

than the human intracranial arteries (around 2 to 5 mm), and two MCAs emerge from the ICA in each hemisphere of the pig, unlike human anatomy. In a pivotal paper, Carniato *et al.* (17) reported an animal model for in vivo evaluation of neuroendovascular devices based on the porcine brachial artery in the flexed forelimb position, which is to replicate the clinically challenging tortuosity of the human ICA at the carotid siphon. Following the reported protocol for the porcine brachial artery tortuosity model (see Materials and Methods for details), we evaluated our system's steering and navigation performances in the porcine brachial artery with accentuated tortuosity in the maximally flexed position, as presented in Fig. 7 and movie S6.

First, a series of images of the target vasculature in the right forelimb were obtained from 3D rotational angiography while injecting the contrast agent through a 7-Fr guide catheter positioned in the brachial branch of the subclavian artery in the flexed forelimb position (Fig. 7A). The acquired images were then reconstructed into a 3D vessel model (Fig. 7B), which allowed for a detailed view of the vascular structure from different perspectives (movie S7) for preprocedural planning. On the basis of the reconstructed 3D vessel model, a semi-anteroposterior projection was chosen to provide clear views of all the side branches (numbered in Fig. 7, B and D) present along the target path in the brachial artery, through the C-arm configuration with cranial angulation of 4° and left anterior oblique rotation of 34° (Fig. 7C). Then, digital subtraction angiography was performed to visualize the target vasculature on the live fluoroscopy images from the chosen projection (movie S6). Note that the vessel roadmap was taken from the angiography data and graphically overlaid on top of the fluoroscopic images in Fig. 7D for clear representation and that the guidewire contour was highlighted to make it clearly visible in the small panels of the figure (movie S7 for raw data).

The first two side branches (1 and 2 in Fig. 7, B and D) in the proximal brachial artery were located at the acute-angled corners, into which the straight tip of the guidewire would have naturally been directed if it were not steered by the externally applied magnetic fields. To prevent the guidewire tip from entering the undesired branch at each corner, the position and orientation of the actuating magnet were identified such that the guidewire tip could be steered toward the desired path, using the 3D vessel model implemented in the virtual task space of the robot arm for real-time visualization and motion planning (Fig. 7E). The corresponding end-effector pose and the configuration of the robot arm were prescribed so that the actuating magnet could readily be positioned upon the operator's command from the remote-control console to steer the magnetic guidewire, as shown in Fig. 7 (D to F) (00:06 to 00:20) and movie S6 (00:00 to 00:30). To demonstrate selective navigation in different branches in the distal area, the magnet pose was prescribed such that the guidewire tip could be steered to selectively reach branches 4 and 5 consecutively, as shown in Fig. 7 (D to F) (00:45 to 01:04) and movie S6 (00:30 to 01:05). Last, the guidewire tip was advanced into the tortuous area with a 360° turn followed by another sharp turn before the goal location. The guidewire tip was initially directed toward the entering curve of the 360° turn, repelled sideways at the 90° corner to make its shape favorable for the sharp turn, and then advanced until it reached the goal, as shown in Fig. 7 (D to F) (01:33 to 01:37) and movie S6 (01:04 to 01:41). Note that the x-ray fluoroscopy was intermittently stopped while repositioning the robot arm, as can be seen in movie S6, to minimize the

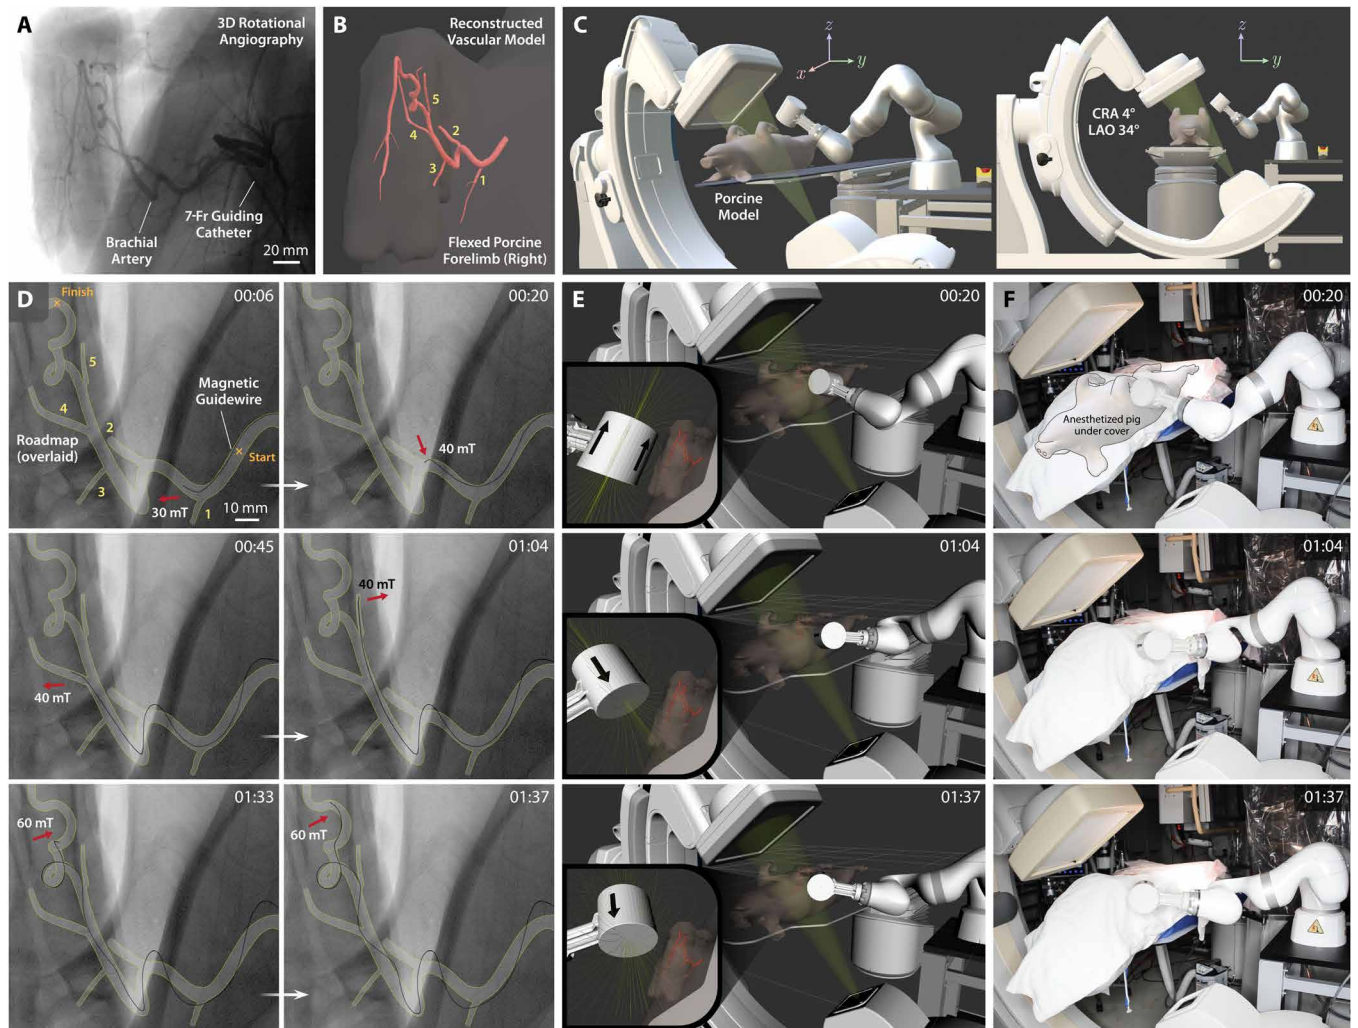


Fig. 7. In vivo demonstration of telerobotically controlled magnetic navigation in porcine brachial artery. (A) Three-dimensional rotational angiography of the porcine brachial artery with accentuated tortuosity in the maximally flexed forelimb position to replicate the tortuosity of the human carotid siphon. (B) Reconstructed 3D model of the target vasculature viewed from a semi-AP projection with all the side branches along the path clearly shown and numbered. (C) Graphical representation of the experimental setup with the C-arm configuration for the chosen semi-AP projection based on cranial angulation of 4° (CRA 4°) and left anterior oblique rotation of 34° (LAO 34°). (D) Fluoroscopic images of the magnetic guidewire navigating in the target vasculature under telerobotically controlled magnetic steering avoiding entering undesired branches (1 and 2) at the acute-angled corners (00:06 to 00:20). The guidewire was steered to selectively reach the side branches (4 and 5) present on the path (00:45 to 01:04) and then reach the goal after negotiating the tortuous region with 360° and 90° turns (01:33 to 01:37). (E) Real-time visualization of the robot arm in a virtual environment simulating the physical testing setup including the C-arm and the anesthetized pig on the operating table. The target vasculature and the magnetic field lines around the actuating magnet are also visualized in real time to enable preprocedural planning of the robot arm's motion for spatial positioning of the magnet relative to the target vasculature. (F) Actual view of the robot arm positioning the magnet based on the prescribed magnet position and orientation for the steering and navigational task upon the operator's command from the remote-control console. Out of respect for the animal and to comply with the Institutional Animal Care and Use Committee policy on photography of research animals, the pig was covered during the video recording. Demonstration of the entire navigation and steering control procedures is available in movie S6. The average time (\pm SD) it took for the demonstrated task was 124.6 ± 19.7 s ($n = 5$).

radiation exposure to the animal as well as the staff present in the catheterization laboratory.

One noticeable difference observed from the in vivo testing above was that the guidewire in the proximal area tended to deviate more greatly from the vessel roadmap as it proceeded more distally along the path, as shown in Fig. 7D, which was rarely observed in the silicone vessels during our in vitro phantom studies presented earlier. This can be attributed to the deformation of the soft blood vessels due to the stiff guidewire, which normally occurs during endovascular navigation with standard guidewires. Nonetheless, the

deformation of the proximal vessels had no effect on the steering of the distal tip of the magnetic guidewire. Except for this apparent deviation of the guidewire from the roadmap, the behavior of the magnetic guidewire in the tortuous porcine brachial artery during the steering and navigational task in vivo was close to that observed in the silicone phantoms, in terms of the device performance and characteristics such as steerability, lubricity, and durability.

No adverse biological or physiological responses such as thrombosis or complications due to endothelial injury such as vessel dissection or perforation were observed during the demonstrated

steering and navigational task in vivo. In addition, no adverse events were observed because of the presence of the magnetic field during the setup, use, and completion of the experiment. These results validate the safety and effectiveness of the telerobotically controlled magnetic steering and navigation in complex and tortuous vasculature in realistic in vivo conditions.

Usability testing and learning curve assessment

Our system allows the operator to remotely control the magnetic guidewire by manipulating the actuating magnet through the robot arm while advancing/retracting the guidewire along with the microcatheter for endovascular navigation and intervention. Although the primary role of the magnetic guidewire is the same as that of conventional ones, in terms of enabling access to the target lesion to initiate interventional procedures, the way in which the magnetic guidewire is manipulated for steering purposes is quite different from the manually controlled passive guidewires based on the twisting maneuver. Hence, new users must be trained to learn how to drive the robot arm and the advancing units with the given teleoperation interface to be able to manipulate the magnetic guidewire and microcatheter under feedback from real-time imaging and visualization.

To assess the learning curve and evaluate the user experience, we conducted a pilot study with six participants who had no prior experiences with the developed telerobotic manipulation platform. The novice group consisted of two engineers with expertise in robotically assisted image-guided therapy and four experienced neurointerventionalists. For this learning curve assessment, we used the 3D neurovascular phantom that was used for the aneurysm coiling and clot retrieval demonstrations in Figs. 5 and 6 in the catheterization laboratory equipped with a standard neurointerventional angiography suite (fig. S15, A and B). The given task for learning curve assessment was endovascular navigation along the previously demonstrated path in Fig. 5, from the left proximal ICA to the inferior M2 segment of the left MCA, as shown in fig. S15C. Learning curves were obtained by tracking procedural time taken for the defined task as a metric for performance over 15 consecutive trials for each participant. Before data collection from the novice group, procedural time was measured from two experienced users (over 15 consecutive trials for each) for comparison. As shown in fig. S15D, the experienced group displayed relatively consistent performance with small deviations over the repeated trials. On average, it took 47.8 ± 12.2 s (mean \pm SD) for the experienced group to complete the given task. The novice group was trained by the experienced users to learn the magnetic steering principles. As part of the training curriculum, each novice performed three practice runs to familiarize themselves with real-time teleoperation of the system under the guidance of the experienced users before starting to track the procedural time.

The average learning curve of the novice group is presented in fig. S15E, with the individual learning curves presented as well in fig. S16, where each dataset was fitted with a logarithmic curve. The average learning curve was short, exhibiting fast decay of the measured time over the number of completed trials. On average, the novice group was able to reduce the procedural time by half after around 5 trials and reach the similar proficiency level of the experienced group after around 12 trials (fig. S15E). The average of the entire trials ($n = 90$; 15 trials from each of the six novices) was 92.8 ± 61.7 s, which was almost double that of the experienced group with much greater deviations. One of the main difficulties

faced by the novices while performing the given task was the presence of the large aneurysm at the acute-angled corner in the carotid siphon, which imposed a navigational challenge that turned out to be the main rate-limiting factor. Although the guidewire tip was seemingly directed correctly toward the desired branch (C4; see Fig. 5A), it tended to exit the desired branch and inadvertently fall into the aneurysm upon further advancement of the guidewire when the actuating magnet was wrongly positioned or oriented, producing insufficient repulsive steering torque. This navigational challenge, however, became manageable after a few trials and could eventually be overcome by every participant, leading to the time reduction. The average of the last 5 trials of the novice group ($n = 30$; last 5 trials from each of the six novices) was 50.1 ± 17.4 s, which was close to the average procedural time (47.8 ± 12.2 s) of the experienced group ($n = 30$; 15 trials from each of the two experienced users). We found no statistically significant difference between the two datasets from Welch's *t* test (two-sample *t* test assuming unequal variances). These results verify that our designed system requires a relatively short period of time for new users to learn how to navigate clinically challenging anatomy with the magnetic guidewire through real-time teleoperation of the robot arm and the advancing unit.

Comparison with conventional guidewires

Last, we evaluated the steering and navigational performance of our telerobotically controlled magnetic guidewire in comparison with that of a manually manipulated conventional guidewire by an experienced neurointerventionalist as shown in Fig. 8A. For comparison, the interventionalist performed the same navigational task in fig. S15C using a standard 0.014-inch (360- μ m) neurovascular guidewire (Synchro 2, Stryker) with a shapeable tip for steering purposes (Fig. 8, B and C). The time it took for the interventionalist to complete the task was measured over 10 consecutive trials (Fig. 8D and movie S7). Before measuring time, the interventionalist was given several practice trials to familiarize himself with the given vascular anatomy and to produce steady-state performances for fair comparison.

One of the navigational challenges encountered was the acutely angled left carotid siphon with a large aneurysm (aneurysm 1 in Fig. 8B), where the 90°-angled tip of the guidewire frequently failed to pass the sharp corner because of the presence of large open space inside the aneurysm (movie S7). Crossing this corner with the pre-shaped guidewire was successful only in 5 trials (trials 3, 4, 5, 6, and 10 in movie S7) of the 10 consecutive trials. In those five successful trials, however, the guidewire's prebent tip was prone to fall into the posterior communicating artery (fig. S8A) upon further advancement after passing the aneurysm, which was unintended. When the guidewire continuously failed to cross the corner (trials 1, 2, 7, 8, and 9 in movie S7), the interventionalist chose to loop the guidewire in the aneurysm to access the desired branch. However, this guidewire looping maneuver can be potentially dangerous, especially in ruptured or in partially thrombosed aneurysms due to the risk of bleeding or displacement of thrombus (33). We also noticed that the prebent tip of the guidewire occasionally latched onto a small aneurysm (aneurysm 2 in Fig. 8B) located at the distal end of the supraclinoid (C4) ICA, as can be seen in Fig. 8F (00:42) and movie S7 (00:16 in trial 5 and 00:42 in trial 7). At the MCA bifurcation with another aneurysm (aneurysm 3 in Fig. 8B), the pre-shaped guidewire also frequently failed to access the desired inferior M2 branch, encountering a similar navigational challenge due to the presence of an aneurysm at the acutely angled corner in six trials

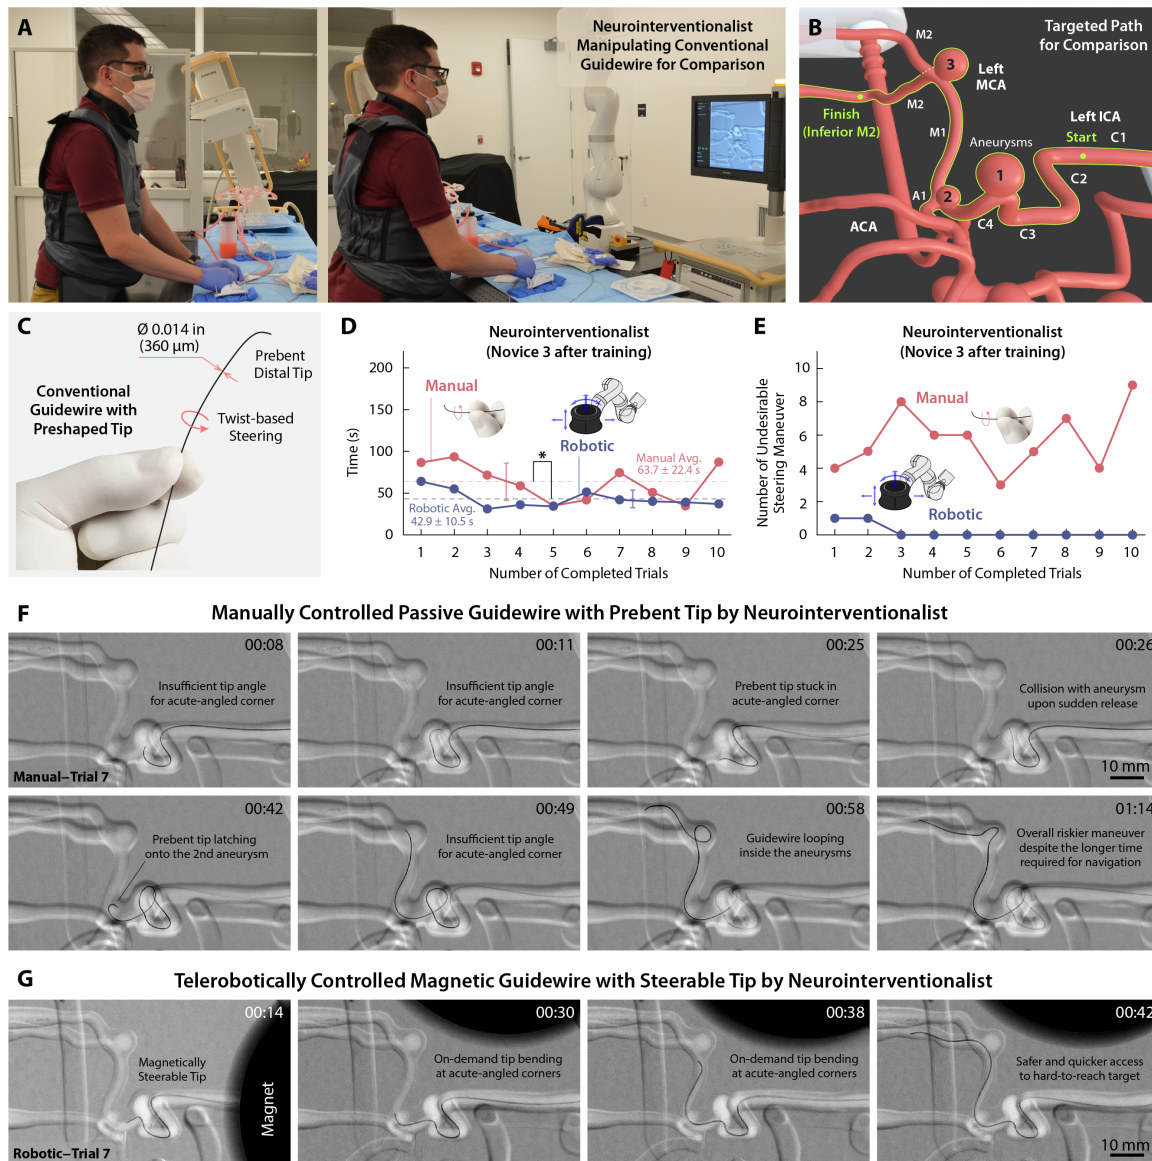


Fig. 8. Evaluation of the steering and navigational performance of the telerobotically controlled magnetic guidewire in comparison with the conventional neurovascular guidewire based on manual manipulation by a neurointerventionalist. (A) Neurointerventionalist manually manipulating a conventional neurovascular guidewire with prebent distal tip for twist-based steering under real-time x-ray fluoroscopy. (B) Defined navigational task for the performance comparison from the left ICA to the inferior M2 segment of the MCA. (C) Conventional neurovascular guidewire (Synchro 2, Stryker) with an outer diameter of 0.014 inches (360 μ m) and prebent (shapeable) distal tip. (D) Comparison of the procedural time (average \pm SD) for the trained neurointerventionalist to complete the defined navigational task using the manually controlled passive guidewire and the telerobotically controlled magnetic guidewire over 10 consecutive trials ($n = 10$) for each experiment. Error bars with whiskers indicate the SD of the measured time, and statistically significant differences are indicated with asterisks ($*P < 0.05$). The interventionalist has +4 years of training and experiences in endovascular neurointervention based on conventional guidewire manipulation and was trained with the telerobotic manipulation system for less than 1 hour (see novice 3 in fig. S16). (E) The number of incidents with undesirable guidewire behavior such as the distal tip colliding with or looping inside aneurysms or falling into undesired branches during the given navigational task. (F) The prebent tip of the conventional guidewire tended to undergo unpredictable and undesirable motion while making frequent contact with the aneurysms present along the path due to the limited steering capability based on twisting maneuver. (G) The magnetic guidewire demonstrated smooth navigation in the narrow and tortuous pathways without any unintended distal tip movement or contact with the aneurysms along the navigated path due to its active steering. Videos for comparison of the steering and navigational performance are available in movies S7 and S8.

(trials 3, 4, 5, 7, 8, and 10 in movie S7). In these six trials, accessing the desired branch required another potentially risky looping maneuver to pass the corner with the aneurysm, as shown in Fig. 8F (00:58 to 01:14). Overall, the manually controlled passive guidewire showed somewhat unpredictable behavior in those clinically challenging

areas, causing several unintended or undesirable incidents such as the guidewire tip colliding with aneurysms, looping inside aneurysms, or falling into undesired branches. The number of such undesirable events encountered while manually manipulating the guidewire was counted for each trial as presented in Fig. 8E.

Unlike the manually controlled passive guidewire, the telerobotically controlled magnetic guidewire enabled access to the clinically challenging branches without requiring a dangerous looping maneuver in the aneurysm sac and obviated unexpected or unintended guidewire tip movements, as can be seen in Fig. 8 (E and G), and movie S8. Overall, the average time to complete the given task was shorter with the telerobotically controlled magnetic guidewire (42.9 ± 10.5 s) when compared with the manually controlled passive guidewire (63.7 ± 22.4 s), and we found statistically significant difference in the procedural time between the two approaches ($P < 0.05$) during the 10 consecutive trials. We assessed the operator's workload in each trial using the NASA Task Load Index (34) as presented in fig. S17. We found statistically significant ($P < 0.05$) reduction in the operator's workload in terms of the mental demand, temporal demand, performance, effort, and frustration with the telerobotically controlled magnetic guidewire when compared with the manually controlled passive guidewire.

These experimental results with quantitative comparison data demonstrate that the telerobotically controlled magnetic guidewire can help to reduce the procedural time as well as the potential risk of vascular perforation or aneurysm rupture while allowing for the operator to work remotely to minimize the radiation exposure. The results also indicate that the telerobotically controlled magnetic navigation could be more predictable and less dependent on the experience and skill of the operator when compared with the manually controlled passive guidewire. This performance comparison was conducted by only one interventionalist, and hence, further studies based on a multiuser trial will be required to confirm the comparison results. Nonetheless, given the technical challenges and functional limitations inherent in conventional guidewires with shapeable/preshaped distal tips, we believe that the demonstrated steering and navigational capabilities of our telerobotic neurointerventional system suggest its potential for improving the quality of endovascular neurosurgery by enabling safer and quicker access to hard-to-reach lesions in the complex neurovasculature.

DISCUSSION

In this work, we have introduced a telerobotic neurointerventional platform with a 7-DOF robot arm used for steering control of the magnetic guidewire and a set of motorized linear drives for precise control of the guidewire or microcatheter advancement, which are controlled remotely under visual feedback from real-time imaging. In the series of benchtop testing, we have shown that our system performs as intended in simulated clinical environments representing the human neurovascular anatomy with clinically challenging tortuosity and disease states such as multiple aneurysms and vascular occlusions. Through the preclinical testing, we have also demonstrated the safety and effectiveness of our developed system for its use in realistic in vivo conditions as well. We have further demonstrated our system's ability to assist therapeutic procedures for endovascular treatments of aneurysms and ischemic stroke in difficult-to-reach areas of cerebral arteries with clinically challenging anatomies. To the best of our knowledge, such telerobotically assisted aneurysm coil embolization and clot retrieval thrombectomy in the complex cerebral vasculature have not been demonstrated with previously reported vascular robotic systems in the literature including the commercial ones discussed earlier (5, 9–16, 35–39). The series of demonstrations here have validated the quantitative analyses

presented in Fig. 3 and fig. S3 for determining the right size of the actuating magnet for clinical use. Further increasing the size of the actuating magnet may allow greater safety margins in terms of its working distance, but the use of a larger magnet would likely affect the flexibility and dexterity of the robot arm mainly because of the greater constraints in terms of the available workspace in cluttered environments. Because it is known that the magnetic susceptibility of biological tissues in the human head causes a negligible effect (below 1%) on the actuating field strength (40), the magnet size verified from the series of benchtop verification would likely be applicable to clinical scenarios.

The concept of magnetically guided intravascular devices has existed for decades (41–46). Despite the long and checkered history of using magnetism to direct intravascular devices (5), there are currently no viable magnetic guidewire/catheter products or commercially available robotic systems to magnetically manipulate such devices for neurovascular applications, where the active steering capability is most needed. Several magnetic guidewire products were introduced for coronary and peripheral interventions in the past by Stereotaxis Inc., in the form of “magnet-tipped” guidewires with a small magnet attached to the distal end tip (5, 38, 39, 47). There have been some similar variants proposed in the research domain, with a few magnets embedded in the distal portion of the guidewire (35). Such magnet-tipped guidewires, however, entail potential risks of embolization because the magnet at the end could break off (48). Furthermore, lacking the ability to conform to the given environment, the rigid and stiff tip of magnet-tipped guidewires could make it particularly challenging to work through narrow and winding pathways in the distal cerebral vasculature. The use of finite-sized, rigid magnets in a thin, flexible device often leads to discontinuous dimensions or mechanical properties along the magnet-tipped guidewire (36), which could substantially compromise its compatibility with other standard interventional devices (e.g., balloon catheters or microcatheters) that are indispensable for the endovascular treatment of aneurysms or stroke.

Magnetic actuation based on a multi-DOF robot arm with a single magnet has been explored in previous studies for different applications such as magnetic capsule endoscopes (49–54). Although the underlying mechanism of using magnetic torques and forces for device control is similar, the hardware design and control strategies of the previously reported systems are specific to their devices based on rigid, finite-sized magnets and hence not directly applicable to steering control of our magnetic continuum guidewire. When it comes to magnetic actuation systems of other types, there are commercialized platforms based on either a pair of large permanent magnets (such as Niobe and Genesis of Stereotaxis Inc.) or a set of multiaxial electromagnets (such as Magnetecs CGCI System and Aeon Phocus), which have been used mostly for cardiac electrophysiology to treat arrhythmia using magnetically controlled ablation catheters. Although these commercialized systems could be used to control our magnetic guidewires, given the previously reported results based on magnet-tipped guidewires (5, 38, 39, 47), such heavy and bulky, hence immobile, platforms may not be ideal for endovascular neurosurgery, especially in the context of telestroke services. Furthermore, for the existing magnetic actuation systems, the available angulation for the monoplane C-arm is limited because of the confined space between the magnets—for example, the Niobe system allows only 28° for the rotation of the C-arm in left or right anterior oblique projection (5). When compared with these

existing magnetic actuation systems, our compact single arm-based platform allows much wider C-arm rotation angles for better state observation as demonstrated in the series of benchtop and preclinical evaluations. Our developed platform based on a compact, lightweight robot arm could therefore suggest a cost-efficient alternative to those existing magnetic navigation systems in realizing robotic telesurgery for stroke intervention.

As demonstrated in figs. S13 and S14 (with related discussions presented in the Supplementary Materials), our telerobotic neuro-interventional system is also compatible with standard biplane fluoroscopy based on a pair of C-arms for simultaneous projections from two different angles. Although single-plane imaging sufficed for most of the navigational tasks demonstrated here, biplanar imaging offered benefits when identifying complex angulations of intracranial vessels as illustrated in figs. S13 and S14. Although monoplane fluoroscopy can be used for stroke interventions, biplane imaging in general could provide better state observation of the guidewire in more complex vascular anatomies and hence potentially improve the operator's confidence, thereby leading to reduced intraoperative risk (55, 56). In this light, biplane imaging may be used when our system is operated in comprehensive stroke centers or tertiary hospitals that are equipped with biplane angiography suites. Note, however, that primary care centers in rural areas are not necessarily equipped with biplane systems mainly because of higher acquisition and maintenance costs. Recent studies (55–57) have shown that experienced neurointerventionalists can perform complex endovascular procedures such as mechanical thrombectomy equally safely and effectively on monoplane systems by using angulation or rotation of the C-arm as they do the same procedures on biplane systems. For these reasons, in the context of telerobotic stroke intervention, we envision that our system could allow the experienced interventionalists at large institutions to perform surgical tasks remotely on patients at their local hospitals that are equipped with monoplane fluoroscopy systems.

There are some potential technical and logistical issues to consider for further translation of our proposed concept and developed system into the clinic. First, communication delays are inevitable in teleoperation systems because of signal propagation time and bandwidth constraints. Because our telerobotic system does not involve any dynamic motion of the robot arm, communication delays are nearly imperceptible to a human operator teleoperating the system from the remote-control console, which is a few meters away from the robot arm. For long-distance intervention in a robotic telesurgery scenario, however, the increased latency may negatively affect the steering control and navigational performance of our system. A recent study reported telerobotically assisted percutaneous coronary intervention in human patients that was performed remotely (32 km away) using the CorPath GRX system under reliable network connection (58). The measured network delay was around 50 ms, and the authors reported that the delay did not result in any noticeable procedural or technical difficulties. We expect that advances in low-latency telecommunications (such as 5G wireless network) and improvements in network connectivity (59, 60) would help to realize long-distance telerobotic stroke intervention (2, 15) when combined with our system. Contingency plans must also exist for periprocedural complications to ensure the feasibility of remotely performed interventions through our proposed system. Although the critical components of endovascular procedures can be performed remotely by a skilled neurointerventionalist (off-site expert) from another hospital, other personnel

on-site will need to be present in the operating room for perioperative assistance from establishing vascular access and handling the C-arm machine to addressing any potential problems or complications that may arise before, during, or after the intervention (2, 3). In this light, the emerging telepresence or teleproctoring systems based on low-latency, high-resolution streaming technology, such as the Tegus system (61, 62), will greatly benefit both off-site and on-site interventionalists by enabling bidirectional communication as well as high-resolution image transmission for real-time fluoroscopic images and visualization of robot configuration.

Second, similarly to other commercial vascular robotic systems with linear drives for guidewire and catheter advancement, the advancing unit of our system does not provide any tactile or haptic feedback. Although the lack of tactile or haptic feedback is often considered one of the major drawbacks of existing vascular robotic systems (9), it should be noted that interventionalists rely mostly on visual feedback when manually manipulating a conventional guidewire. Some recent studies support this standpoint, reporting that the lack of tactile feedback in the CorPath GRX system did not result in any procedural challenges or adverse clinical outcomes (13, 14), mainly because of the ability to detect obstacles and friction visually by observing subtle changes in the shape and motion of the guidewire. Likewise, we believe that the tactile feedback may not be a critical factor for telerobotically performed endovascular navigation because the system provides the ability to stop advancing or retracting the guidewire and microcatheter immediately when the operator observes any undesirable behavior of the device from real-time fluoroscopic imaging. Nonetheless, we believe that the implementation of force-sensing and haptic feedback technologies would help to improve the control interface and operator performance (3), which is therefore an area for future exploration.

From the presented *in vitro* and *in vivo* studies here, we found that preoperative imaging (3D rotational angiography and reconstructed 3D vessel models) can play a pivotal role in preprocedural planning of the robot arm's motion, path, and configuration for spatial positioning of the actuating magnet to steer the magnetic guidewire at critical locations such as branching points or sharp corners in the target vasculature. We envision that preplanned robot motion for spatial positioning of the actuating magnet based on the preoperative imaging data can help to make the system easier for interventionalists to use by reducing the operator's workload in real-time teleoperation of the robot arm with a joystick controller. This preprocedural planning will also be crucial for future developments of the proposed robotic neurointerventional platform toward semiautonomous or fully autonomous endovascular navigation in the complex neurovasculature based on magnetic manipulation. In doing so, model-based estimation and control of the magnetic soft continuum guidewire under the action of a single actuating magnet will also be an important area for future development, given the practical constraints on real-time 3D shape sensing and tracking capabilities due to the projected challenges in miniaturizing sensors or reconstructing the 3D guidewire shapes from the standard mono- or biplane x-ray fluoroscopic images.

MATERIALS AND METHODS

Telerobotic magnetic manipulation platform

A kinematically redundant, serial robotic manipulator with seven revolute joints (LBR Med 14 R820, KUKA) was used to manipulate

a N52-grade cylindrical magnet ($B_{re} = 1.45$ T) with diameter and thickness of 100 mm (Hangzhou X-mag Inc.), which was mounted on the flange of the robot arm using a 3D-printed magnet housing. The net weight of the magnet and the fixture was 7 kg, and the center of the mass was 160 mm away from the robot arm's flange at the most distal link. The strength of the magnetic field from the magnet at this distance from the flange did not affect the position and torque sensors at each joint of the robot arm. The magnetic field and field gradient maps around the actuating magnet presented in figs. S3A and S4 were generated using a commercial finite element analysis software (COMSOL Multiphysics 5.2). The teleoperation control interface was designed on the basis of the open-source libraries and tools such as MoveIt (for control of the robot arm based on the joint commands $\delta\mathbf{q}$ computed from Eq. 6 and motion planning with collision avoidance) and RViz (graphical interface for real-time visualization of the robot arm) available in the Robot Operating System (ROS). A joystick controller with a 6-DOF knob (SpaceMouse Pro Wireless, 3Dconnexion) was used for remote control of the robot end effector for spatial positioning of the magnet.

Guidewire/microcatheter advancing unit

A pair of cylindrical brushed DC gearmotors with integrated encoders (High-power 12 V, Pololu) was used to build the guidewire and microcatheter advancing units. Along with the DC motors, a motor driver (Dual VNH5019 Motor Driver Shield, Pololu) and a microcontroller board (Arduino Uno R3) were assembled in a 3D-printed motor housing (Fig. 2A). A pair of catheter advancers (QuikCAS Cardiodrive, Stereotaxis Inc.) was connected to the DC motors through flexible shafts to advance or retract the guidewire and the microcatheter, each of which was coupled to a 7-Fr introducer sheath/dilator (Destination Guiding Sheath, Terumo) through a straight hemostasis valve connector (Qosina). The control interface for the guidewire/microcatheter advancing unit based on manipulation of the joystick buttons was implemented in the ROS environment to build an integrated teleoperation interface for the system.

In vitro testing setup

For demonstrations presented in figs. S7 and S10 to S13 and movie S1, a 3D neurovascular model based on silicone vessels (Trandomed) was used. For demonstrations presented in Fig. 4, fig. S14, and movie S2, a human head phantom with cranial housing (Vascular Simulations Inc.) was used for realistic simulation of workspace constraints due to patient geometry. These anatomical models included both carotid and vertebral arteries and a complete circle of Willis in realistic dimensions. Multiple aneurysms with different neck morphologies, sizes, and angulations from the carrier vessel were present on these anatomical models (figs. S8 and S14). The silicone vessels were filled with a blood-mimicking fluid (Replicator Fluid, Vascular Simulations Inc.), along with a peristaltic pump to generate pulsatile flow, to simulate the friction between commercial hydrophilic guidewire/catheter surfaces and the real blood vessels. To demonstrate the repeatability of the navigational task in Fig. 4 and movie S2, the experiment was repeated five times to evaluate the average time taken for completion and the SD. To compare the interventionist's performance with the telerobotically controlled magnetic guidewire and the manually controlled passive guidewire (Fig. 8 and movies S7), a standard neurovascular guidewire (Synchro 2, Stryker) with a shapeable tip and an outer diameter of 0.014 inches (360 μm) was used. During the comparison, the operator's task load was also assessed

via the NASA Task Load Index to compare the experienced task load from the two different approaches (fig. S17).

Telerobotically assisted therapeutic procedures

For the demonstrations of aneurysm coil embolization presented in Fig. 5 with movie S3 and in fig. S10 with movie S4, bare platinum coils with an outer diameter of 0.0115 inches (290 μm) (Axium Prime, Medtronic) were used. For the demonstration of clot retrieval thrombectomy presented in Fig. 6 with movie S5 and fig. S11, a stent retriever device (Solitaire X Revascularization Device, Medtronic) was used to retrieve a simulated clot (ASIST Thrombus Simulant, Vascular Simulation Inc.). To create the occlusion in the left, a cylindrical plug of the thrombus simulant was deposited in the left ICA through an 8-Fr guide catheter with an inner diameter of 2.9 mm (Destination Guiding Sheath, Terumo), and then a peristaltic pump was turned on to generate a pulsatile flow that carried the thrombus up to the M1 segment. A rotating hemostatic valve (Qosina) was connected to the microcatheter hub to tighten or loosen the introducer sheath of the embolization coils or the stent retriever when transferring those therapeutic devices into the microcatheter.

In vivo animal testing setup

A female Yorkshire swine of 56 kg was used for our animal testing. All procedures were conducted in accordance with the protocol approved by the Institutional Animal Care and Use Committee of University of Massachusetts Medical School and the Committee on Animal Care of Massachusetts Institute of Technology. Following the previously reported protocol (17), the swine was anesthetized and maintained with mechanical ventilation under continuous monitoring of its physiologic status. A 10-Fr hemostatic introducer (Check-Flo Performer Introducer, Cook Medical) was placed in the right femoral artery by using a modified Seldinger technique. A 0.035-inch (889- μm) diagnostic guidewire (Glidewire, Terumo) was manually manipulated under x-ray fluoroscopy to reach the brachial branch of the right subclavian artery, and a 7-Fr guide catheter (Destination Guiding Sheath, Terumo) was advanced manually over the diagnostic guidewire to be placed in the proximal brachial artery for contrast injection and angiography. After removing the diagnostic guidewire, the magnetic guidewire was then advanced up to the proximal brachial artery to initiate the preclinical evaluation of magnetic steering and navigation through real-time teleoperation of the robot arm and the guidewire advancing unit.

Characterization of magnetic steering control

For the characterization data presented in Fig. 3C and figs. S5B and S6B, the guidewire's tip deflection angle θ was experimentally measured from the images taken with a high-resolution camera (acA2440-35uc, Basler AG) while varying the distance d , the angular position ϕ , and the rotation angle α of the actuating magnet of cylindrical shape with diameter and thickness of 76.2 mm relative to the steerable tip. The distal portion of the magnetic guidewire was clamped and fixed with a nonmagnetic miniature gripper (Mark-10) to impose a fixed boundary condition while exposing only the distal 10-mm segment of the magnetically responsive tip that was free to deflect under the influence of the actuating magnet (Fig. 3B).

Statistical analyses

To demonstrate the repeatability of the in vitro navigation presented in Fig. 4 with movie S2 and fig. S12 and the in vivo navigation

presented in Fig. 7 with movie S6, each of the experiments was repeated five times to evaluate the average and SD of the time it took to complete the navigational task. Similarly, for repeatability of the telerobotically performed therapeutic procedures presented in Fig. 5 with movie S3, Fig. 6 with movie S5, and fig. S10 with movie S4, each of the experiments was repeated three times to evaluate the average and SD of the time it took for the demonstrated procedure. Welch's *t* test (two-sample *t* test assuming unequal variances) was performed to verify that there was no statistically significant difference in the performance between the experienced users and the trained novices, when comparing the average procedural time of the last 5 trials of the novice group ($n = 30$; last 5 trials from each of the six novices) with that of the experienced group ($n = 30$; 15 trials from each of the two experienced users) in fig. S15E. For the data presented in Fig. 8D with movies S7 and S8 to compare the steering and navigational performance of the manually controlled passive guidewire and the telerobotically controlled magnetic guidewire, each of the experiments was repeated 10 times to evaluate the average and SD of the time it took for the interventionalist to complete the given task. In Fig. 8D and fig. S17, statistically significant differences are indicated with asterisks ($*P < 0.05$) based on the *P* values obtained from paired *t* tests (two-sample *t* test for means).

SUPPLEMENTARY MATERIALS

www.science.org/doi/10.1126/scirobotics.abg9907

Supplementary Text

Figs. S1 to S17

Movies S1 to S8

Reference (63)

REFERENCE AND NOTES

- S. S. Virani, A. Alonso, E. J. Benjamin, M. S. Bittencourt, C. W. Callaway, A. P. Carson, A. M. Chamberlain, A. R. Chang, S. Cheng, F. N. Delling, L. Djousse, M. S. V. Elkind, J. F. Ferguson, M. Fornage, S. S. Khan, B. M. Kissela, K. L. Knutson, T. W. Kwan, D. T. Lackland, T. T. Lewis, J. H. Lichtman, C. T. Longenecker, M. S. Loop, P. L. Lutsey, S. S. Martin, K. Matsushita, A. E. Moran, M. E. Mussolino, A. M. Perak, W. D. Rosamond, G. A. Roth, U. K. A. Sampson, G. M. Satou, E. B. Schroeder, S. H. Shah, C. M. Shay, N. L. Spartano, A. Stokes, D. L. Tirschwell, L. B. VanWagner, C. W. Tsao; American Heart Association Council on Epidemiology and Prevention Statistics Committee and Stroke Statistics Subcommittee, Heart disease and stroke statistics—2020 update: A report from the American Heart Association. *Circulation* **141**, e139–e596 (2020).
- S. S. Panesar, J. J. Volpi, A. Lumsden, V. Desai, N. S. Kleiman, T. L. Sample, E. Elkins, G. W. Britz, Telerobotic stroke intervention: A novel solution to the care dissemination dilemma. *J. Neurosurg.* **132**, 971 (2019).
- M. Goyal, G. R. Sutherland, S. Lama, P. Cimflova, N. Kashani, A. Mayank, M.-N. Psychogios, L. Spelle, V. Costalat, N. Sakai, J. M. Ospel, Neurointerventional robotics: Challenges and opportunities. *Clin. Neuroradiol.* **30**, 203–208 (2020).
- U.S. Food and Drug Administration (FDA), Center for Devices and Radiological Health, *Coronary, Peripheral, and Neurovascular Guidewires – Performance Tests and Recommended Labeling* (FDA-2018-D-1775, 2019); www.fda.gov/regulatory-information/search-fda-guidance-documents/coronary-peripheral-and-neurovascular-guidewires-performance-tests-and-recommended-labeling.
- T. Krings, J. Finney, P. Niggemann, P. Reinacher, N. Lück, A. Drexler, J. Lovell, A. Meyer, R. Sehra, P. Schauer, M. Reinges, F. J. Hans, A. Thron, Magnetic versus manual guidewire manipulation in neuroradiology: In vitro results. *Neuroradiology* **48**, 394–401 (2006).
- M. R. Harrigan, J. P. Deveikis, *Handbook of Cerebrovascular Disease and Neurointerventional Technique* (Humana Press, 2012).
- C. E. Hoffer, A. M. Ilyas, Fluoroscopic radiation exposure: Are we protecting ourselves adequately? *J. Bone Joint Surg. Am.* **97**, 721–725 (2015).
- Y. Kim, G. A. Parada, S. Liu, X. Zhao, Ferromagnetic soft continuum robots. *Sci. Robot.* **4**, eaax7329 (2019).
- S. A. Menaker, S. S. Shah, B. M. Snelling, S. Sur, R. M. Starke, E. C. Peterson, Current applications and future perspectives of robotics in cerebrovascular and endovascular neurosurgery. *J. Neurointerv. Surg.* **10**, 78–82 (2018).
- J. Bonatti, G. Vetrovec, C. Riga, O. Wazni, P. Stadler, Robotic technology in cardiovascular medicine. *Nat. Rev. Cardiol.* **11**, 266–275 (2014).
- J. Troccaz, G. Dagnino, G.-Z. Yang, Frontiers of medical robotics: From concept to systems to clinical translation. *Annu. Rev. Biomed. Eng.* **21**, 193–218 (2019).
- J. Chakravartti, S. V. Rao, Robotic assisted percutaneous coronary intervention: Hype or hope? *J. Am. Heart Assoc.* **8**, e012743 (2019).
- V. M. Pereira, N. M. Cancelliere, P. Nicholson, I. Radovanovic, K. E. Drake, J.-M. Sungur, T. Krings, A. Turk, First-in-human, robotic-assisted neuroendovascular intervention. *J. Neurointerv. Surg.* **12**, 338–340 (2020).
- G. W. Britz, J. Tomas, A. Lumsden, Feasibility of robotic-assisted neurovascular interventions: Initial experience in flow model and porcine model. *Neurosurgery* **86**, 309–314 (2020).
- K. C. Sajja, A. Sweid, F. Al Saiegh, N. Chalouhi, M. B. Avery, R. F. Schmidt, S. I. Tjoumakaris, M. R. Gooch, N. Heriati, R. Abbas, H. Zarzour, V. Romo, R. Rosenwasser, P. Jabbour, Endovascular robotic: Feasibility and proof of principle for diagnostic cerebral angiography and carotid artery stenting. *J. Neurointerv. Surg.* **12**, 345–349 (2020).
- V. M. Pereira, P. Nicholson, N. M. Cancelliere, X. Y. E. Liu, R. Agid, I. Radovanovic, T. Krings, Feasibility of robot-assisted neuroendovascular procedures. *J. Neurosurg.* , 1–13 (2021).
- S. Carniato, M. Mehra, R. M. King, A. K. Wakhloo, M. J. Gounis, Porcine brachial artery tortuosity for in vivo evaluation of neuroendovascular devices. *Am. J. Neuroradiol.* **34**, E36–E38 (2013).
- S. Chiaverini, G. Oriolo, I. D. Walker, Kinematically redundant manipulators, in *Springer Handbook of Robotics*, B. Siciliano and O. Khatib, Eds. (Springer Nature, 2008), pp. 245–268.
- Y. Kim, H. Yuk, R. Zhao, S. A. Chester, X. Zhao, Printing ferromagnetic domains for untethered fast-transforming soft materials. *Nature* **558**, 274–279 (2018).
- R. Zhao, Y. Kim, S. A. Chester, P. Sharma, X. Zhao, Mechanics of hard-magnetic soft materials. *J. Mech. Phys. Solids* **124**, 244–263 (2019).
- L. Wang, Y. Kim, C. F. Guo, X. Zhao, Hard-magnetic elastica. *J. Mech. Phys. Solids* **142**, 104045 (2020).
- ASAHI Neurovascular Guide Wire Instruction for Use (Asahi Intecc, 2012); <https://asahi-inteccusa-medical.com/wp-content/uploads/2019/07/ASAHI-IFU-Neurovascular-Guidewire.pdf>.
- Z. Zhuang, B. Bradtmiller, Head-and-face anthropometric survey of U.S. respirator users. *J. Occup. Environ. Hyg.* **2**, 567–576 (2005).
- D. J. Craik, *Magnetism: Principles and Applications* (Wiley, 1995).
- J. S. Agashe, D. P. Arnold, A study of scaling and geometry effects on the forces between cuboidal and cylindrical magnets using analytical force solutions. *J. Phys. D Appl. Phys.* **41**, 105001 (2008).
- C. D. Natali, M. Beccani, P. Valdastris, Real-time pose detection for magnetic medical devices. *IEEE Trans. Magn.* **49**, 3524–3527 (2013).
- K. M. Lynch, F. C. Park, *Modern Robotics: Mechanics, Planning, and Control* (Cambridge Univ. Press, 2017).
- S. Torikoshi, Y. Akiyama, A concealed intracranial aneurysm detected after recanalization of an occluded vessel: A case report and literature review. *Interv. Neurol.* **4**, 90–95 (2016).
- T. Krings, D. M. Mandell, T.-R. Kiehl, S. Geibprasert, M. Tymianski, H. Alvarez, K. G. Terbrugge, F.-J. Hans, Intracranial aneurysms: From vessel wall pathology to therapeutic approach. *Nat. Rev. Neurol.* **7**, 547–559 (2011).
- R. M. Starke, A. Turk, D. Ding, R. W. Crowley, K. C. Liu, N. Chalouhi, D. M. Hasan, A. S. Dumont, P. Jabbour, C. R. Durst, R. D. Turner, Technology developments in endovascular treatment of intracranial aneurysms. *J. Neurointerv. Surg.* **8**, 135–144 (2016).
- ASIST Proprietary Thrombus Simulant (Vascular Simulations, 2020); <https://vascularsimulations.com/simulation-accessories/#thrombus>.
- F. Arikian, T. Martínez-Valverde, Á. Sánchez-Guerrero, M. Campos, M. Esteves, D. Gandara, R. Torné, L. Castro, A. Dalmau, J. Tibau, J. Sahuquillo, Malignant infarction of the middle cerebral artery in a porcine model. A pilot study. *PLoS ONE* **12**, e0172637 (2017).
- A. von Hessling, T. Reyes del Castillo, G. Karwacki, J. E. Roos, The Columbus steerable guidewire in neurointerventions: Early clinical experience and applications. *J. Neurointerv. Surg.* **14**, 291–296 (2021).
- A. P. Mamunes, F. Campisano, J. Martin, B. Scaglioni, E. Mazomenos, P. Valdastris, K. L. Obstein, Magnetic flexible endoscope for colonoscopy: An initial learning curve analysis. *Endosc. Int. Open* **09**, E171–E180 (2021).
- S. Jeon, A. K. Hoshiar, K. Kim, S. Lee, E. Kim, S. Lee, J.-Y. Kim, B. J. Nelson, H.-J. Cha, B.-J. Yi, H. Choi, A magnetically controlled soft microrobot steering a guidewire in a three-dimensional phantom vascular network. *Soft Robot.* **6**, 54–68 (2018).
- A. Azizi, C. C. Tremblay, K. Gagné, S. Martel, Using the fringe field of a clinical MRI scanner enables robotic navigation of tethered instruments in deeper vascular regions. *Sci. Robot.* **4**, eaax7342 (2019).
- S. Jeong, Y. Chitalia, J. P. Desai, Design, modeling, and control of a coaxially aligned steerable (COAST) guidewire robot. *IEEE Robot. Autom. Lett.* **5**, 4947–4954 (2020).
- M. Schiemann, R. Killmann, M. Kleen, N. Abolmaali, J. Finney, T. J. Vogl, Vascular guide wire navigation with a magnetic guidance system: Experimental results in a phantom. *Radiology* **232**, 475–481 (2004).
- K. Tsuchida, H. M. García-García, W. J. van der Giessen, E. P. McFadden, M. van der Ent, G. Sianos, H. Meulenbrug, A. T. L. Ong, P. W. Serruys, Guidewire navigation in coronary

- artery stenoses using a novel magnetic navigation system: First clinical experience. *Catheter. Cardiovasc. Interv.* **67**, 356–363 (2006).
40. J. J. Tharayil, S. M. Goetz, J. M. Bernabei, A. V. Peterchev, Field distribution of transcranial static magnetic stimulation in realistic human head model. *Neuromodulation* **21**, 340–347 (2018).
 41. H. Tillander, Magnetic guidance of a catheter with articulated steel tip. *Acta Radiol.* **35**, 62–64 (1951).
 42. J. F. Alksne, Magnetically controlled intravascular catheter. *Surgery* **64**, 339–345 (1968).
 43. J. Molcho, H. Z. Karny, E. H. Frei, H. M. Askenasy, Selective cerebral catheterization. *I.E.E.E. Trans. Biomed. Eng.* **17**, 134–140 (1970).
 44. H. L. Cares, J. R. Hale, D. B. Montgomery, H. A. Richter, W. H. Sweet, Laboratory experience with a magnetically guided intravascular catheter system. *J. Neurosurg.* **38**, 145–154 (1973).
 45. S. K. Hilal, W. J. Michelsen, J. Driller, E. Leonard, Magnetically guided devices for vascular exploration and treatment. *Radiology* **113**, 529–540 (1974).
 46. M. S. Grady, M. A. Howard, R. G. Dacey, W. Blume, M. Lawson, P. Werp, R. C. Ritter, Experimental study of the magnetic stereotaxis system for catheter manipulation within the brain. *J. Neurosurg.* **93**, 282–288 (2000).
 47. S. Ramcharitar, M. S. Patterson, R. J. van Geuns, C. van Meighem, P. W. Serruys, Technology insight: Magnetic navigation in coronary interventions. *Nat. Clin. Pract. Cardiovasc. Med.* **5**, 148–156 (2008).
 48. U.S. Food and Drug Administration (FDA), *Class 2 Medical Device Recalls: Cronus Endovascular Guidewires* [510(K) Number: K021363, FDA, 2004]; www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfRES/res.cfm?start_search=1&number=K021363.
 49. A. W. Mahoney, J. J. Abbott, Five-degree-of-freedom manipulation of an untethered magnetic device in fluid using a single permanent magnet with application in stomach capsule endoscopy. *Int. J. Rob. Res.* **35**, 129–147 (2016).
 50. L. B. Kratchman, T. L. Bruns, J. J. Abbott, R. J. Webster, Guiding elastic rods with a robot-manipulated magnet for medical applications. *IEEE Trans. Robot.* **33**, 227–233 (2017).
 51. A. Z. Taddese, P. R. Slawinski, M. Pirota, E. De Momi, K. L. Obstein, P. Valdastrì, Enhanced real-time pose estimation for closed-loop robotic manipulation of magnetically actuated capsule endoscopes. *Int. J. Rob. Res.* **37**, 890–911 (2018).
 52. G. Pittiglio, L. Barducci, J. W. Martin, J. C. Norton, C. A. Avizzano, K. L. Obstein, P. Valdastrì, Magnetic levitation for soft-tethered capsule colonoscopy actuated with a single permanent magnet: A dynamic control approach. *IEEE Robot. Autom. Lett.* **4**, 1224–1231 (2019).
 53. J. C. Norton, P. R. Slawinski, H. S. Lay, J. W. Martin, B. F. Cox, G. Cummins, M. P. Y. Desmulliez, R. E. Clutton, K. L. Obstein, S. Cochran, P. Valdastrì, Intelligent magnetic manipulation for gastrointestinal ultrasound. *Sci. Robot.* **4**, eaav7725 (2019).
 54. J. W. Martin, B. Scaglioni, J. C. Norton, V. Subramanian, A. Arezzo, K. L. Obstein, P. Valdastrì, Enabling the future of colonoscopy with intelligent and autonomous magnetic manipulation. *Nat. Mach. Intell.* **2**, 595–606 (2020).
 55. C. A. Bellemare, T. G. Poder, Effectiveness of biplane angiography compared to monoplane angiography for vascular neuro-interventions: A systematic review of the literature. *Clin. Radiol.* **72**, 6121.e1–6125.e5 (2017).
 56. B. Friedrich, C. Maegerlein, D. Lobsien, S. Mönch, M. Berndt, D. Hedderich, S. Wunderlich, D. Michalski, M. Lehm, T. Boeckh-Behrens, C. Zimmer, K. Kreiser, Endovascular stroke treatment on single-plane vs. bi-plane angiography suites. *Clin. Neuroradiol.* **29**, 303–309 (2019).
 57. A. Guenego, P. J. Mosimann, M. Wintermark, J. J. Heit, K. Zuber, T. Dobrocky, J. A. Lotterie, P. Nicholson, D. G. Marcellus, J. M. Olivot, N. Gonzalez, R. Blanc, V. M. Pereira, J. Gralla, J. Kaesmacher, R. Fahed, M. Piotin, C. Cognard, E. Piechowiak, P. Mordasini, F. Zibold, C. Ducroux, F. Bonneville, J. Darcourt, I. Vukasinovic, A. C. Januel, S. Monfrais, C. Michelozzi, P. Tall, M. Mazighi, J.-P. Desilles, G. Ciccio, S. Smajda, H. Redjem, B. Maier, B. W. Martin, E. Guenego, F. Carbillat, Safety and effectiveness of neuro-thrombectomy on single compared to biplane angiography systems. *Sci. Rep.* **10**, 4470 (2020).
 58. T. M. Patel, S. C. Shah, S. B. Pancholy, Long distance tele-robotic-assisted percutaneous coronary intervention: A report of first-in-human experience. *EClinicalMedicine* **14**, 53–58 (2019).
 59. X. Jiang, H. Shokri-Ghadikolaei, G. Fodor, E. Modiano, Z. Pang, M. Zorzi, C. Fischione, Low-latency networking: Where latency lurks and how to tame it. *Proc. IEEE* **107**, 280–306 (2019).
 60. J. Zheng, Y. Wang, J. Zhang, W. Guo, X. Yang, L. Luo, W. Jiao, X. Hu, Z. Yu, C. Wang, L. Zhu, Z. Yang, M. Zhang, F. Xie, Y. Jia, B. Li, Z. Li, Q. Dong, H. Niu, 5G ultra-remote robot-assisted laparoscopic surgery in China. *Surg. Endosc.* **34**, 5172–5180 (2020).
 61. M. Bechstein, J.-H. Buhk, A. M. Frölich, G. Broocks, U. Hanning, M. Erler, M. Andelkovic, D. Debeljak, J. Fiehler, E. Goebell, Training and supervision of thrombectomy by remote live streaming support (RESS): Randomized Comparison Using Simulated Stroke Interventions. *Clin. Neuroradiol.* **31**, 181–187 (2019).
 62. M. Bechstein, S. Elsheikh, F. Wodarg, C. A. Taschner, U. Hanning, J.-H. Buhk, R. McDonough, E. Goebell, J. Fiehler, M. Bester, Republished: Interhospital teleproctoring of endovascular intracranial aneurysm treatment using a dedicated live-streaming technology: first experiences during the COVID-19 pandemic. *J. Neurointerv. Surg.* **13**, e1 (2020).
 63. H. Gibo, C. Lenkey, A. L. Rhoton, Microsurgical anatomy of the supraclinoid portion of the internal carotid artery. *J. Neurosurg.* **55**, 560–574 (1981).

Acknowledgments: We thank S. U. Lee and H. Bowman (Massachusetts Institute of Technology) for helpful discussion and feedback on the manuscript. We also thank A. Patriciu and S. Kyne (Philips Research) for participating in usability testing and learning curve assessment and providing feedback and M. Flexman and A. Gupta (Philips Research) for insightful discussion and constructive feedback on the developed system. We also thank C. Thammavong (Massachusetts General Hospital) for help with fluoroscopic imaging and R. King, E. Langan, C. Brooks, and M. Gounis (University of Massachusetts Medical School) for help with animal testing. **Funding:** This work was supported by the National Science Foundation (EFRI-1935291) and NIH (1R01HL153857-01) and funded in part by Philips Research North America through MIT-Philips research alliance. Y.K. acknowledges the financial support through a scholarship from IJUU Academy and Culture Foundation and MIT School of Engineering MathWorks Fellowship. **Author contributions:** Y.K. and X.Z. conceived and designed the study. Y.K. developed the magnetic soft continuum guidewire and the telerobotic manipulation platform and its control interface. Y.K. and E.G. developed the guidewire/catheter advancing unit and its control interface. Y.K., J.C., P.H., and M.B. conducted the in vitro experiments and analyzed the results. P.H. and A.B.P. provided guidance and feedback on the demonstrated endovascular interventional procedures. Y.K., J.C., M.B., and R.W.R. conducted the in vivo animal study and analyzed the results. Y.K., J.C., P.H., M.B., R.W.R., J.E.V., A.A.D., and A.B.P. conducted the usability testing for learning curve assessment and provided feedback. P.H. evaluated the performance of the telerobotically controlled magnetic guidewire in comparison with the manually controlled passive guidewire and assessed the operator's task load. Y.K. and X.Z. wrote the manuscript with input from all authors. X.Z. supervised the study. **Competing interests:** Y.K. and X.Z. are listed as inventors of a patent on the presented telerobotic neurointerventional system and the magnetic soft continuum guidewire. The other authors declare that they have no competing financial interests. **Data and materials availability:** All data are provided in the manuscript and the Supplementary Materials and are available online in <https://doi.org/10.5061/dryad.8pk0p2nq8>.

Submitted 8 February 2021
 Accepted 17 March 2022
 Published 13 April 2022
 10.1126/scirobotics.abg9907

Telerobotic neurovascular interventions with magnetic manipulation

Yoonho Kim, Emily Genevriere, Pablo Harker, Jaehun Choe, Marcin Balicki, Robert W. Regenhardt, Justin E. Vranic, Adam A. Dmytriw, Aman B. Patel, and Xuanhe Zhao

Sci. Robot. **7** (65), eabg9907. DOI: 10.1126/scirobotics.abg9907

View the article online

<https://www.science.org/doi/10.1126/scirobotics.abg9907>

Permissions

<https://www.science.org/help/reprints-and-permissions>

Use of this article is subject to the [Terms of service](#)

Science Robotics (ISSN 2470-9476) is published by the American Association for the Advancement of Science, 1200 New York Avenue NW, Washington, DC 20005. The title *Science Robotics* is a registered trademark of AAAS.

Copyright © 2022 The Authors, some rights reserved; exclusive licensee American Association for the Advancement of Science. No claim to original U.S. Government Works